

# Smart Sensing for Antibiotic Monitoring in Mineral and Surface Water: Development of an Electronic Tongue Device <sup>†</sup>

Cátia Magro <sup>1,\*</sup>, Tiago Moura <sup>1</sup>, Paulo A. Ribeiro <sup>2</sup>, Maria Raposo <sup>2</sup> and Susana Sérgio<sup>2,\*</sup>

<sup>1</sup> Department of Physics, NOVA School of Science and Technology, NOVA University Lisbon, 2829-516 Caparica, Portugal; ta.moura@campus.fct.unl.pt (T.M.)

<sup>2</sup> Laboratory of Instrumentation, Biomedical Engineering and Radiation Physics (LIBPhys-UNL), Department of Physics; NOVA School of Science and Technology, NOVA University Lisbon, 2829-516 Caparica, Portugal; pfr@fct.unl.pt (P.A.R.); mfr@fct.unl.pt (M.R.)

\* Correspondence: c.magro@fct.unl.pt (C.M.); susana.serio@fct.unl.pt (S.S.)

<sup>†</sup> Presented at the 1st International Electronic Conference on Chemical Sensors and Analytical Chemistry, 01–15 July 2021; Available online: <https://csac2021.sciforum.net/>.

**Abstract:** Sensors are considered the future monitoring tools since compared to traditional sampling and analysis techniques, they provide fast response on the output data in a timely, continuous, safe, and cost-effective fashion. The antibiotics are important pharmaceuticals with a large variety of applications. However, the over-consumption of these drugs is under the spotlight, since traces of antibiotics are being found in aquatic ecosystems and may lead to the development of antibiotic resistance. Thus, in this work, sensors consisting of ceramic or glass BK7 solid supports with interdigitated gold electrodes coated with 5 bilayers of polyethyleneimine (PEI) and poly(sodium 4-styrenesulfonate) (PSS) thin films were developed and able to distinguish clarithromycin concentrations, between  $10^{-15}$  M and  $10^{-5}$  M, in mineral and surface water matrices. In the mineral water, the ceramic support sensors have shown high reproducibility, whereas glass support sensors are not reproducible for this matrix. For the surface water matrix, both types of sensors proved to be reproducible. The surface water's principal component analysis, obtained for an electronic tongue composed of the aforementioned sensors, demonstrated the concept's ability to discriminate between different concentrations of the target compound, although no significant pattern of trend was achieved.

**Keywords:** environmental monitoring; antibiotics; clarithromycin; electronic tongue; impedance spectroscopy

**Citation:** Magro, C.; Moura, T.; Ribeiro, P.A.; Raposo, M.; and Sérgio, S.; Smart sensing for antibiotic monitoring in mineral and surface water: development of an electronic tongue device. *Chem. Proc.* **2021**, *3*, x. <https://doi.org/10.3390/xxxxx>

Published: 5 July 2021

**Publisher's Note:** MDPI stays neutral with regard to jurisdictional claims in published maps and institutional affiliations.



**Copyright:** © 2021 by the authors. Submitted for possible open access publication under the terms and conditions of the Creative Commons Attribution (CC BY) license (<http://creativecommons.org/licenses/by/4.0/>).

## 1. Introduction

Antibiotic consumption has grown substantially since their discovery and represents an important class of pharmaceuticals employed for treating bacterial infections by killing bacteria or preventing it from spreading. Antimicrobial drugs are widely utilized in human and veterinary medicine, as well as in agriculture [1]. Although these chemicals allow us to live longer and have healthier lives, their over-consumption poses a great threat, mainly regarding the development of antibiotic resistance [2].

Clarithromycin is a macrolide, a class of antibiotic drugs produced by multiple *streptomyces* strains, mostly effective against gram-positive bacteria [3]. It is paramount to understand the occurrence and fate of macrolides in the environment since traces of these drugs are frequently detected in surface and ground waters. Accordingly, the European Commission included clarithromycin, together with other macrolides, in the 2<sup>nd</sup> Watch List of Emerging Water Pollutants. This surface water Watch List was developed with the

purpose of obtaining high-quality monitoring data regarding several potential water pollutants to establish their environmental and health risks, therefore emphasizing the importance of developing efficient techniques to detect and quantify such pollutants.

Analytical methods based on liquid chromatography (LC) and mass spectrometry (MS) provide low detection limits, but require intensive sample preparation, expensive equipment, experienced operators, and are not designed for *in situ* analysis [4,5]. The sensors are considered the future of monitoring tools and present many advantages compared to traditional techniques [6]. Sensor devices are low cost, simple to operate and can be used for continuous, fast and reliable *in situ* monitoring [7–9]. Even, sensors are not as selective as LC/MS methods, they have proved to be able to identify multiple analytes simultaneously [6].

The electronic tongue (e-tongue) refers to a device that consists of an array of non-specific chemical and/or physical sensors that display cross-sensitivity to target compounds in a liquid matrix [10]. E-tongue devices may rely on potentiometry, voltammetry or impedance spectroscopy as transducing methods [11].

The present work aims to explore the potential of the e-tongue concept to monitor different clarithromycin concentrations, relying on the discussion of the reproducibility of an array of sensors coated with PEI/PSS thin films in two different environmental aqueous matrices: mineral and surface water.

## 2. Materials and Methods

Clarithromycin (Sigma-Aldrich, Steinheim, Germany) solutions with concentrations between  $10^{-15}$  M and  $10^{-5}$  M were prepared by sequential dilutions of a mother solution with a concentration of  $10^{-4}$  M. All dilutions, as well as the mother solution, were prepared with experimental matrix/MeOH (9:1) solutions. The experimental matrices utilized to prepare the solutions were a commercial Portuguese mineral water (MW) and a surface water (SW) collected from Tagus River at Porto Brandão, Caparica, Portugal. Lastly, solutions without clarithromycin, containing only experimental matrix/MeOH (9:1), were prepared for the MW and SW matrices to be used as the blank standard (0 M).

The sensors used in this work consist of interdigitated gold electrodes (IDE) deposited on ceramic and glass BK7 solid supports purchased from DropSens (Oviedo, Asturias, Spain). The dimensions of the ceramic support are 22.8 mm × 7.6 mm × 1 mm, the width of each “finger” and the spacing between “fingers” are both 200 μm. The glass supports’ dimensions are 22.8 mm × 7.6 mm × 0.7 mm and the width of each “finger”, like the spacing between “fingers”, is 10 μm. The sensor devices were coated with thin films of polyethyleneimine (PEI) and poly(sodium 4-styrenesulfonate) (PSS) produced by the layer-by-layer (LbL) technique [12]. The substrates were alternately immersed in positively and negatively charged polyelectrolyte solutions with concentrations of  $10^{-2}$  M for 30 s. After the adsorption of each layer, the substrates were immersed in water in order to remove any polyelectrolyte molecules that were not completely adsorbed. At the end of the deposition of each bilayer, the substrates were dried with nitrogen gas stream (99% purity, Air Liquide, Algés, Portugal). The thin films of PEI/PSS were prepared with 5 bilayers, (PEI/PSS)<sub>5</sub>.

The electrical analysis was achieved by impedance spectroscopy measurements of the sensor devices when immersed in aqueous matrices spiked with different clarithromycin concentrations. The impedance spectra were obtained with a Solartron 1260 Impedance Analyzer (Solartron Analytical, AMETEK scientific instruments, Berwyn, PA, USA) in the frequency range of 1 Hz to 1 MHz by applying an alternate voltage with an amplitude of 25 mV.


The principal component analysis (PCA) was performed, regarding the normalized (Z-Score normalization  $\frac{value - \mu}{\sigma}$ , being  $\mu$  and  $\sigma$ , the mean value and the standard deviation of the samples, respectively) impedance spectroscopy data, to reduce the size of data

and to obtain a new space of orthogonal components, in order to detect and explain different concentration patterns. The clarithromycin detection in the target matrices was further evaluated by an array of sensors, composed by all produced thin films, using the e-tongue concept.

### 3. Results and Discussion


#### 3.1. Sensor Reproducibility

To draw conclusions on the reproducibility of the (PEI/PSS)<sub>5</sub> sensors, each solution of clarithromycin was analyzed with two identical sensors produced under the same conditions. The average of the two sensors' data was calculated as a function of the frequency for each matrix and type of sensor (glass or ceramic support). The standard deviation was used as a measure of the uncertainty. In Figure 1 is depicted the average of the impedance magnitude measured by (a) 2 ceramic support and (b) 2 glass support sensors when immersed in the MW matrix. Figure 1(a) reveals that the ceramic support sensors coated with (PEI/PSS)<sub>5</sub> are reproducible when monitoring clarithromycin in MW, since the values of the standard deviation are small (two orders of magnitude smaller than the average), meaning that the results of both sensors are similar. Furthermore, Figure 1(b) shows that there is a significant discrepancy between the measurements of the two glass support sensors, which results in larger standard deviation values. These results can be explained since the spacing between the IDE "fingers" is smaller in the glass support sensors and thus the electric field generated between them, when an AC voltage signal is applied, has a larger magnitude. Additionally, the MW matrix has a lower conductivity, containing ion species in lower concentrations, affecting, therefore, the interactions between the matrix and the sensor. Consequently, at lower frequency values (< 10 Hz), measurements of the glass sensors immersed in MW are compromised (see Figure 1 (b), region highlighted by a red dashed rectangle).

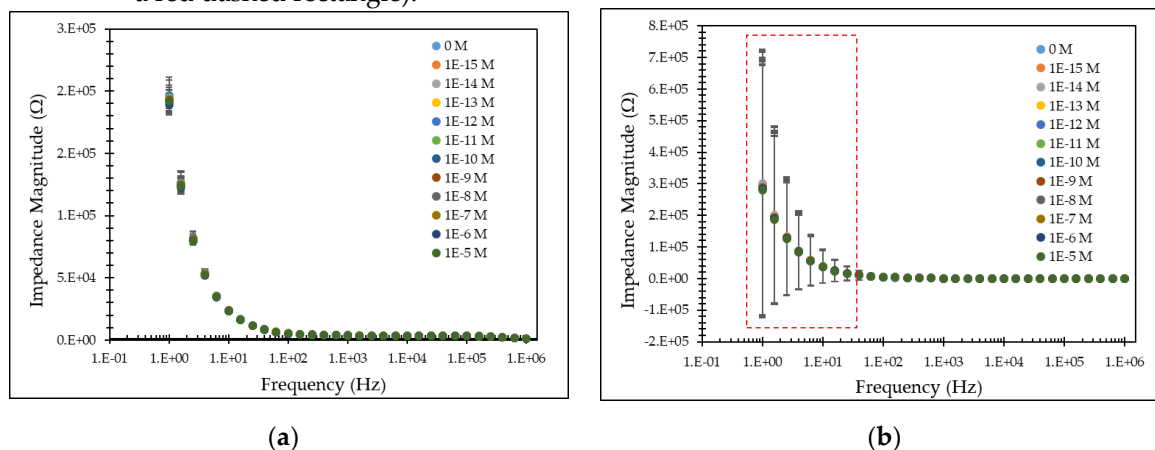

**Figure 1.** Reproducibility of the impedance magnitude measured by (a) 2 ceramic support and (b) 2 glass support sensors in a MW matrix.

Regarding the analysis of clarithromycin solutions prepared with SW, Figure 2(a) and Figure 2(b) show the average of the capacitance measured by 2 ceramic support sensors and 2 glass support sensors, respectively.

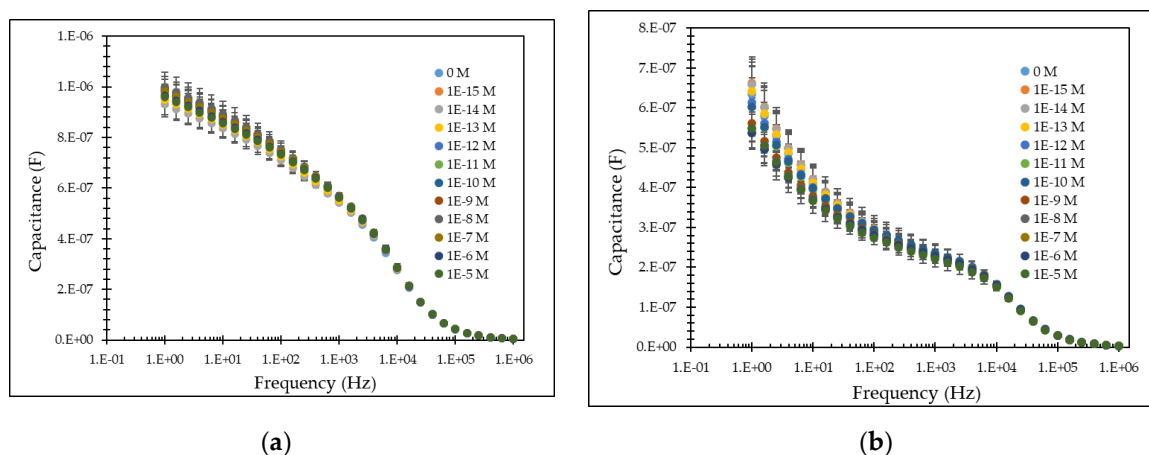


**Figure 2.** Reproducibility of the capacitance measured by (a) 2 ceramic support and (b) 2 glass support sensors in a SW matrix.

Figure 2(a) reveals that there is not a considerable difference between the results of both ceramic sensors. As stated before, this conclusion can be drawn from the low values of the standard deviation ( $10^{-10}$ – $10^{-8}$  F). Figure 2(b) provides similar conclusions, thus both types of sensors show good reproducibility when monitoring SW matrices. However, for the SW matrix, the glass support sensors coated with (PEI/PSS)<sub>5</sub> thin films present a more noticeable sensitivity to discriminate clarithromycin concentrations in the frequency range of 1–100 Hz.

On the other hand, the sensors with a ceramic support showed superior reproducibility for both experimental matrices. Furthermore, the ceramic sensors produced more reliable results in the frequency region of 1–100 Hz for MW. For SW, both types of sensors achieved better reproducibility in the measurements from 1 Hz to 100 Hz.

### 3.2. Principal Component Analysis: e-tongue

The results of the principal component analysis applied to the e-tongue concept will be presented and discussed only for SW. The e-tongue concept was not applied for MW since the glass support sensors were not reproducible as evidenced by the analysis of the impedance electrical characterization (Figure 1b). Thus, Figure 3 displays the PCA plots obtained for an array of sensors composed of 2 ceramic support sensors, for MW (Figure 3 a), and 2 ceramic support sensors combined with 2 glass support sensors for SW (Figure 3 b). In both target matrices, the array of sensors was coated with (PEI/PSS)<sub>5</sub> thin films.

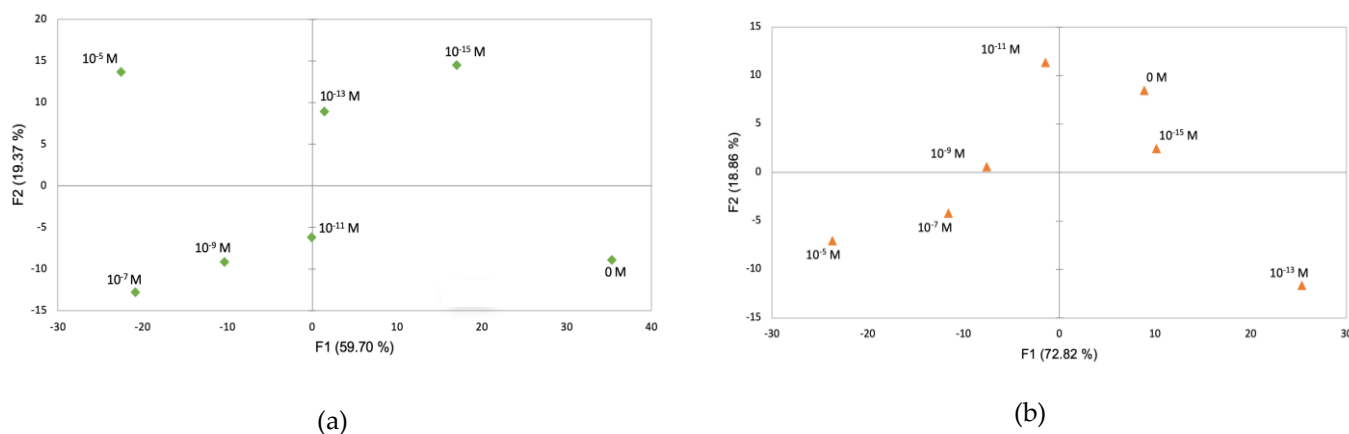

**Figure 3.** PCA plots for clarithromycin concentrations (0– $10^{-5}$  M) discriminated by an e-tongue for (a) MW and (b) SW.

In Figure 3 (a) the first two principal components account for 91.68% of the total variance. The PCA plot reveals that the ceramic support sensors provide the ability to discriminate between different clarithromycin concentrations and the blank solution. It can be also observed a pattern in the concentration decay, with  $10^{-13}$  M as outlier. Figure 3(b) shows the PCA plot for an array of sensors identical to the one discussed above but immersed in SW solutions. In this case, the first two principal components accounted for 79.07% of the total variance. The plot reveals that the e-tongue concept provides the ability to discriminate between non-doped and doped SW solutions. Additionally, the sensors were able to distinguish the different clarithromycin concentrations.

#### 4. Conclusions

Sensors composed of ceramic or glass BK7 solid supports, with interdigitated gold electrodes, were coated with 5 bilayers of PEI/PSS thin films produced by the LbL technique. An electronic tongue consisting of an array of these sensors was shown to provide the ability to distinguish between clarithromycin concentrations in the range of  $10^{-15}$  M to  $10^{-5}$  M in surface water.

The electrical analysis of the samples was performed with impedance spectroscopy by immersing the sensors in the water samples with different clarithromycin concentrations. An average of the measurements obtained with two identical sensors and the associated standard deviation were used to study the reproducibility of the sensors. In the MW matrix, the ceramic sensors showed reproducibility. The opposite can be said for the glass support sensors, which for lower frequencies struggle to identify the target compound. In the SW matrix, both types of sensors, ceramic, or glass support, were proven to be highly reproducible.

Results of the principal component analysis of the impedance data did not show clear pattern or trend but was able to distinguish between doped and non-doped solution, both for MW and SW matrices. To achieve better results, the e-tongue concept requires a wider variety of thin films deposited on the sensors, as, for example, metal oxides or carbon based thin films.

**Author Contributions:** Conceptualization, C.M., T.M, M.R. and S.S.; methodology, T.M.; software, T.M.; validation, C.M., M.R. and S.S.; formal analysis, C.M, M.R. and S.S; investigation, T.M. and C.M.; resources, P.A.R, M.R. and S.S.; data curation, T.M.; writing—original draft preparation, C.M, T.M., M.R. and S.S; writing—review and editing, C.M, , M.R. and S.S; supervision, C.M, , M.R. and S.S; project administration, M.R.; funding acquisition, P.A.R, M.R. and S.S. All authors have read and agreed to the published version of the manuscript.

**Funding:** The research leading to these results has received funding from the Portuguese funding agency FCT—Fundação para a Ciência e a Tecnologia—within projects PTDC/FIS-NAN/0909/2014, UID/FIS/04559/2020 to LIBPhys-UNL from the FCT/MCTES/PIDDAC , and the Bilateral Project entitled “Detecção de Estrogénio- um Contaminante Emergente em Corpos Hídricos” within the scope of “Cooperação Transnacional\_FCT (Portugal)-CAPES (Brazil) 2018”.

**Institutional Review Board Statement:** Not applicable.

**Informed Consent Statement:** Not applicable.

**Acknowledgments:** C. Magro acknowledges NOVA.ID of NOVA-FCT for her postdoc fellowship.

**Conflicts of Interest:** The authors declare no conflict of interest.

#### References

1. Silbergeld, E.K.; Graham, J.; Price, L.B. Industrial food animal production, antimicrobial resistance, and human health. *Annu. Rev. Public Health* **2008**, *29*, 151–169.
2. Zimdahl, R.L. Antibiotics. In *Six Chemicals That Changed Agriculture*; Elsevier: Amsterdam, The Netherlands, 2015; pp. 165–182.
3. Hagren, V.; Peippo, P.; Lövgren, T. Detecting and controlling veterinary drug residues in poultry. In *Food Safety Control in the Poultry Industry*; Mead, G.C., Ed.; Woodhead Publishing Limited: Southston, UK, 2005; pp. 44–82.

4. Zhang, Y.; Zhu, Y.; Zeng, Z.; Zeng, G.; Xiao, R.; Wang, Y.; Hu, Y.; Tang, L.; Feng, C. Sensors for the environmental pollutant detection: Are we already there? *Coord. Chem. Rev.* **2021**, *431*, 213681.
5. Rawtani, D.; Khatri, N.; Tyagi, S.; Pandey, G. Nanotechnology-based recent approaches for sensing and remediation of pesticides. *J. Environ. Manage.* **2018**, *206*, 749–762.
6. Magro, C.; Mateus, E.P.; Fátima Raposo, M.; Ribeiro, A.B. Emerging Contaminants in Wastewater: Sensor Potential for Monitoring Electroremediation Systems. In *Electrokinetic Remediation for Environmental Security and Sustainability*; Wiley: Hoboken, NJ, USA, 2021; pp. 413–432.
7. Ciosek, P.; Wróblewski, W. Sensor arrays for liquid sensing- electronic tongue systems. *Analyst* **2007**, *132*, 963–978.
8. Kruss, S.; Hilmer, A.J.; Zhang, J.; Reuel, N.F.; Mu, B.; Strano, M.S. Carbon nanotubes as optical biomedical sensors. *Adv. Drug Deliv. Rev.* **2013**, *65*, 1933–1950.
9. Barsan, M.M.; Ghica, M.E.; Brett, C.M.A. Electrochemical sensors and biosensors based on redox polymer/carbon nanotube modified electrodes: A review. *Anal. Chim. Acta* **2015**, *881*, 1–23.
10. Vlasov, Y.; Legin, A. Non-selective chemical sensors in analytical chemistry: from “electronic nose” to “electronic tongue.” *Fresenius. J. Anal. Chem.* **1998**, *361*, 255–260.
11. Latha, R.S.; Lakshmi, P.K. Electronic tongue: An analytical gustatory tool. *J. Adv. Pharm. Technol. Res.* **2012**, *3*, 3–8.
12. Oliveira, O.N.; Raposo, M.; Dhanabalan, A. Langmuir-blodgett and self-assembled polymeric films. In *Handbook of Surfaces and Interfaces of Materials*; Nalwa, H.S.B.T.-H. of S. and I. of M., Ed.; Elsevier: Burlington, 2001; pp. 1–63 ISBN 978-0-12-513910-6.