

Innovative method of high sensitivity and separation detection for ciguatoxin analogues by LC-MS/MS

Manami Kobayashi¹; Naomasa Oshiro²

¹Shimadzu Corporation, Kawasaki-city, Japan; ²Division of Biomedical Food Research, National Institute of Health Sciences, Kawasaki-city, Japan

1. Introduction

Ciguatera Fish Poisoning is the world's most prevalent source of food poisoning, and it is caused by ciguatoxins (CTXs), thermostable polyether toxins produced by benthic dinoflagellates. CTXs are found in natural samples in trace amounts, and they pose neurotoxic effects at concentrations as low as 0.2 µg/kg. The US FDA and EFSA recommends a control level of 0.01 µg CTX1B equivalent/kg. Previously published work (Yogi, K. et. al.; *Anal. Chem.* 2011, 83, 8886-8891)¹⁾ using a LC/MS/MS instrument achieved the control levels monitoring the sodium adducts of the targets of interest ([M+Na]⁺ > [M+Na]⁺). In this study, we optimized a highly sensitive method for the detection of CTXs using the sodium and lithium adducts, [M+Na]⁺ and [M+Li]⁺ ions, by adding very small amounts of alkali metals, such as Na⁺ and Li⁺ to the mobile phase. This work demonstrates that CTXs can be successfully detected at the low concentrations recommended by FDA with good chromatographic separation by LC/MS/MS. We report in this poster the new analytical conditions and accuracy of the method using [M+Li]⁺.

2. Materials and Methods

2-1. CTXs reference materials

- qNMR quantified reference materials of five CTX analogs were provided by JFRL (Japan Food Analysis Center)²⁾.
- CTX mix standard solution containing nine CTX analogs was prepared at NIHS (National Institute of Health Science).

2-2. Analytical conditions

The analysis was performed with the LCMS-8060NX coupled with a Nexera™ X3 UHPLC system (Shimadzu Corporation, Kyoto, Japan), following conditions summarized in Table 1.

UHPLC conditions	
Equipment	: Nexera X3 system (Shimadzu Corporation)
Column	: Shim-pack Velox™ C18 (50 mm × 2.1 mm I.D., 1.8 µm)
Mobile phase A	: water/formic acid (1000 : 1, v : v)
Mobile phase B for Na Adduct: acetonitrile/formic acid/0.05 M sodium hydroxide aqueous solution (1000 : 1 : 1, v : v : v)	
Mobile phase B for Li Adduct: acetonitrile/formic acid/0.1 M lithium hydroxide monohydrate solution (1000 : 1 : 1, v : v : v)	
Flow rate	: 0.4 mL/min (0.6 mL/min from 12.01 to 17.0 min)
Time program	: 8 Conc. 40 % (0.0 – 2.5 min) → 85 % (12.0 min) → 100 % (12.01 – 17.0 min) → 40 % (17.01 – 20 min)
Column temperature	: 40 °C
Injection volume	: 5 µL
The flow was loaded into the MS detector between 2.5 to 12.5 min using a flow switching valve.	
MS conditions	
Equipment	: LCMS-8060NX
Ionization	: ESI, Positive MRM mode
IF/ion focus voltage	: +1 / +4 KV
IF/DL/HB temperature	: 350 °C/300 °C/400 °C
Nebulizer gas	: 3 L/min
Heating gas	: 15 L/min
Drying gas	: 5 L/min
CID gas pressure	: 270 Kpa
Collision Energy	: -40 V : CTX1B, 2,3-dihydroxyCTX3C, 52- <i>epi</i> -54-deoxyCTX1B, 54-deoxyCTX1B, 51-hydroxyCTX3C -30 V : 49- <i>epi</i> CTX3C, CTX3C, CTX4A, CTX4B
MRM transition for Na Adduct: [M+Na] ⁺ > [M+Na] ⁺	
m/z	1133.60: CTX1B
m/z	1079.60: 2,3-dihydroxyCTX3C
m/z	1117.60: 52- <i>epi</i> -54-deoxyCTX1B & 54-deoxyCTX1B
m/z	1061.60: 51-hydroxyCTX3C
m/z	1045.60: 49- <i>epi</i> CTX3C & CTX3C
m/z	1083.60: CTX4A & CTX4B
MRM transition for Li Adduct: [M+Li] ⁺ > [M+Li] ⁺	
m/z	1117.60: CTX1B,
m/z	1063.60: 2,3-dihydroxyCTX3C
m/z	1101.60: 52- <i>epi</i> -54-deoxyCTX1B & 54-deoxyCTX1B
m/z	1045.60: 51-hydroxyCTX3C
m/z	1029.60: 49- <i>epi</i> CTX3C & CTX3C
m/z	1067.60: CTX4A & CTX4B



3. Results

3-1. Formation of [M+Na]⁺ or [M+Li]⁺ ion

The addition of Na⁺ or Li⁺ to the mobile phase is known to increase the formation of sodium or lithium adducts through cationization⁴⁾. A trace amount of alkali metal was added to the mobile phase in order to obtain the desired ions, either [M+Na]⁺ or [M+Li]⁺ (Table 1). The specific ions from CTX1B are shown in Fig. 2 (SIM spectra) as an example. Same results were obtained with the other target compounds analyzed in this study. When Li⁺ was added to the mobile phase, [M+Na]⁺ was not detected. These results suggested that enhanced sensitivity could be achieved using alternative ions, such as [M+Li]⁺.

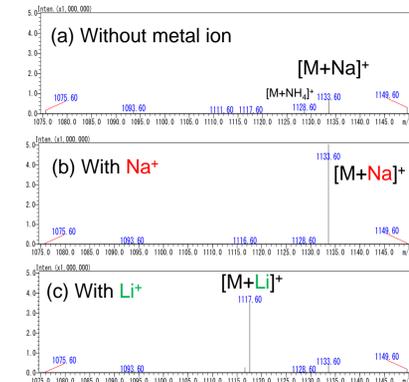


Figure 2 Multi spectra of CTX1B by different mobile phases (SIM).

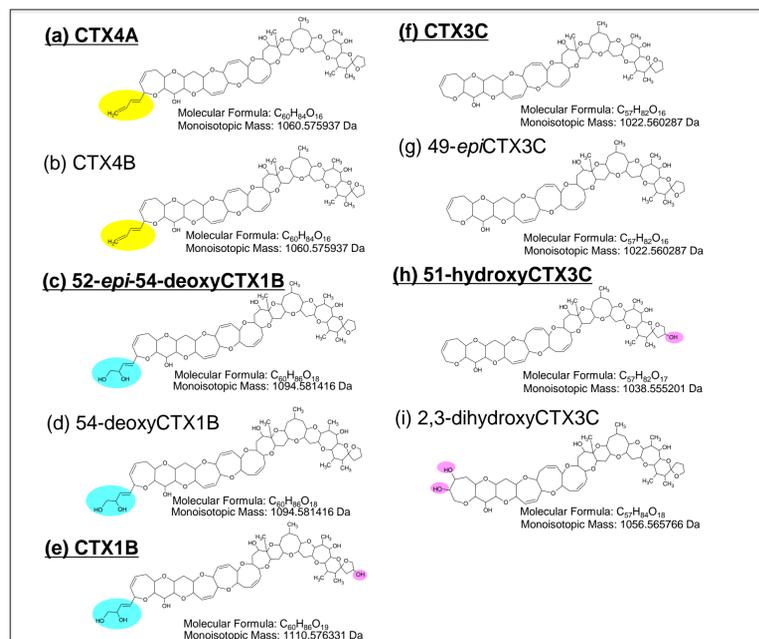


Figure 1. The structure of the nine compounds. JFRL reference materials : (a) CTX4A, (c) 52-*epi*-54-deoxyCTX1B, (e) CTX1B, (f) CTX3C, (h) 51-hydroxyCTX3C

3-2. Optimization of Collision energy (CE)

Unfortunately, [M+Na]⁺ and [M+Li]⁺ precursor ions did not provide any useful product ions. Thus, we optimized the CE to provide the highest S/N when monitor [M+Na]⁺ > [M+Na]⁺ or [M+Li]⁺ > [M+Li]⁺ on MRM analysis mode. Optimized CE for CTX1B are shown in Table 1. The best CE of the remaining 8 analogs were optimized in similar way.

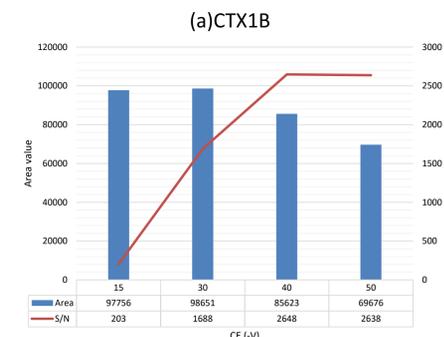


Figure 3 The relationship between the CE and the peak area or S/N.

3-3. Improved peak separation and sensitivity

In Fig. 4 ((a), (b), (c)), separation of the target compounds using previously reported conditions ((a); Oshiro, N. et. al., *J. Mar. Sci. Eng.* 2023, 11, 242)⁵⁾, Na-added mobile phase (b), and Li-added mobile phase (c) is compared. 2,3-dihydroxyCTX3C and 51-hydroxyCTX3C, 49-*epi*-CTX3C and CTX3C, CTX4A and CTX4B showed dramatically better separation under new conditions (Fig. 4 (b)(c)). 6 analogs other than 2,3-dihydroxyCTX3C and 51-hydroxyCTX3C and CTX3C had good sensitivity in Na-added mobile phase. It was confirmed that the sensitivity of the 9 analogs of interest was comparable when using Li-added mobile phases.

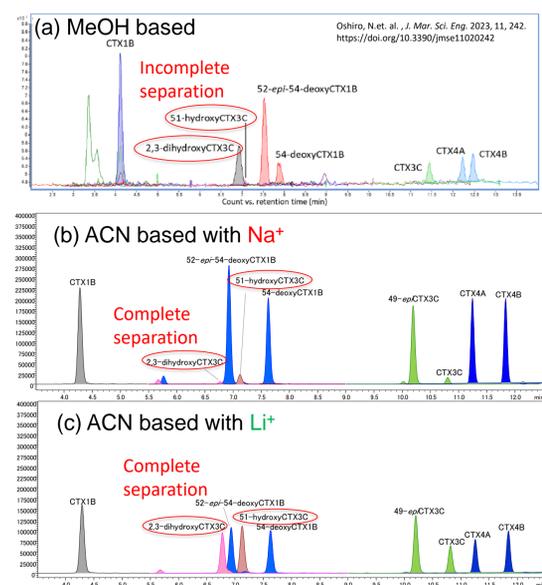


Figure 4 MRM chromatograms of 9 analogues (1 ng/mL NIHS-CTX-Mix ver.2)

3-4. Evaluation of the limit of quantification(LOQ)

Calibration curves were generated using JFRL reference materials to confirm the sensitivity of [M+Li]⁺ > [M+Li]⁺. Each chromatogram at the lowest point of the calibration curve is shown in Figure 5. The range of the calibration curve was determined so that the average Accuracy in 3 replicate analyses of each calibration point was 100±5%, and the lowest point was designated as the LOQ. When 1 mL of the assay solution was prepared from 5 g of fish meat, the LOQs of the five standard substances adopted as the lowest point of the calibration curve in this method ranged from 0.0004 to 0.0012 µg/kg (Table 2).

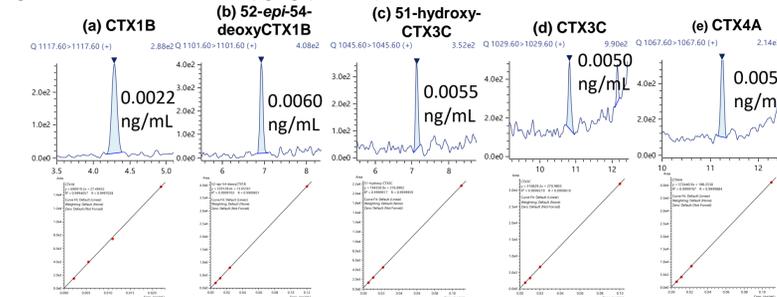


Figure 5 MRM chromatograms of the lowest point of the calibration curve and the calibration curve (JFRL Reference Materials)

Table 2 LOQ, reproducibility and accuracy of each analogue (n=3)

	LOQ (ng/mL)	LOQ (µg/kg)	Retention time (min)	%RSD (Area)	Accuracy (%)	S/N
CTX1B	0.0022	0.0004	4.289	11.02	98	81
52- <i>epi</i> -54-deoxyCTX1B	0.0060	0.0012	6.931	5.38	105	64
51-hydroxy-CTX3C	0.0055	0.0011	7.121	8.76	103	22
CTX3C	0.0050	0.0010	10.815	12.32	102	22
CTX4A	0.0055	0.0011	11.250	17.28	105	36

S/N was calculated by rms method with 0.5 min near the peak as noise.

4. Conclusions

- ✓ The new optimized LC/MS/MS conditions enable sensitivity exceeding the FDA tolerance level for CTXs.
- ✓ These results suggest that a general-purpose LC-MS/MS from any manufacturer can be used for highly sensitive analysis of CTXs.

5. Acknowledgements

We are grateful to Dr. Takeshi Yasumoto for providing the reference materials of CTXs.

6. Reference

- Yogi, K.; Oshiro, N.; Inafuku, Y.; Hiram, M.; Yasumoto, T.; Detailed LC-MS/MS analysis of ciguatoxins revealing distinct regional and species characteristics in fish and causative alga from the Pacific, *Anal. Chem.* 2011, 83, 8886-8891
- Kato T.; Yasumoto T.; Quantification of Representative Ciguatoxins in the Pacific Using Quantitative Nuclear Magnetic Resonance Spectroscopy, *Mar. Drugs* 15, 309 (2017)
- Jia Jun Wu et al.; Validation of an accelerated solvent extraction liquid chromatography–tandem mass spectrometry method for Pacific ciguatoxin-1 in fish flesh and comparison with the mouse neuroblastoma assay, *Anal. Bioanal. Chem.* (2011) 400:3165–3175
- Klijnstra, Mirjam D., and Arjen Gerssen.; A Sensitive LC-MS/MS Method for Palytoxin Using Lithium Cationization, *Toxins* 10, no. 12 (2018): 537
- Oshiro, N. et. al.; Analytical Studies on Ciguateric Fish in Okinawa, Japan (II): The Grouper *Variola albigarginata*, *J. Mar. Sci. Eng.* 2023, 11, 242.

7. Patents

This analytical method is patent pending. PCT/JP2022/045132, 2022-089617(JP)