

Proceeding Paper

Amperometric Ion-Selective Electrodes Based on Prussian Blue Nanoparticles †

Vera Shavokshina¹, Vita Nikitina¹ and Arkady Karyakin¹

¹ Chemistry Department of M.V. Lomonosov Moscow State University, Leninskie Gory, 1/3, Moscow, 119991, Russia

* Correspondence: shavokshinava@my.msu.ru

† Presented at the 2nd International Electronic Conference on Chemical Sensors and Analytical Chemistry, 16-30 September 2023.

Abstract: We report on amperometric solid-contact potassium-selective electrodes based on catalytically synthesized Prussian Blue nanoparticles. Both the films and nanoparticles are able to generate amperometric response in flow-injection mode under constant potential. However, nanoparticles provide higher sensitivity than the films. Moreover, the intrinsic permeability of Prussian blue for potassium ions allows for selective detection of potassium in comparison to sodium even without ion-selective membrane. The results of Electrochemical impedance spectroscopy were used to manage the sensitivity by controlling the charge transfer resistance for ion-selective membranes of different density. By performing measurements in Bis-Tris as a carrier buffer containing no interfering cations an additional increase in selectivity was enabled. The record selectivity coefficient $\log K_{Na^+/K^+}$ is -2.7 for amperometric flow-injection mode was achieved. The obtained results indicate the prospects for analysis of biological fluids since Na^+/K^+ ratio is approximately 20-40.

Keywords: solid-contact; Prussian Blue; Nanoparticles. Flow injection amperometry

1. Introduction

The control of the electrolyte composition of physiological fluids is important in clinical practice, in particular, potassium ions, which are associated with hydration status and involved in muscle contraction. The normal level of potassium in the blood serum is 3.5 to 5.5 mM. Both the lack of ions and their excess have a negative impact on human health [1]. Potentiometric ion-selective electrodes (ISE) became a gold standard in analytical chemistry and are used for quantification of various analytes. The use of a solid contact instead of liquid junction makes it possible to simplify the design of the sensor and reduce its size. In the last decade, the creation of solid contact ion-selective electrodes (SC-ISE) operating in non-zero current mode has attracted interest [2,3].

Previously, we have proposed a fundamentally new approach, alternative to classical potentiometry [4,5], which consists in registration of the current response at a constant potential in flow-injection amperometry mode. This approach eliminates the limitations of potentiometric SC-ISE such as baseline drift and potential instability. Even though conductive organic polymers are commonly utilized as solid contacts, inorganic materials are also a viable option [6].

The zeolite structure of Prussian Blue (PB) allows to entrap the potassium cations [7], this is an advantage for elaborating K^+ -sensitive SC-ISE based on PB. Moreover, SC-ISE using PB as solid contact are already known [8-11]. However, these sensors are capable of detecting sodium ions or provide dual sensing of Na^+ and K^+ ions. Despite the successful application of various PB nanomaterials for cations detection, ISE based on PB nanoparticles has not been reported.

Citation: To be added by editorial staff during production.

Academic Editor: Firstname Last-name

Published: date

Publisher's Note: MDPI stays neutral with regard to jurisdictional claims in published maps and institutional affiliations.



Copyright: © 2022 by the authors. Submitted for possible open access publication under the terms and conditions of the Creative Commons Attribution (CC BY) license (<https://creativecommons.org/licenses/by/4.0/>).

In this work, we develop SC-ISE based on catalytically synthesized PB nanoparticles for potassium detection. The effect of membrane density and carrier buffer used for flow injection analysis (FIA) on sensor performance was studied.

2. Materials and Methods

2.1. Materials

Experiments were carried out with Millipore Milli-Q water. Hydrogen peroxide (30 %) and inorganic salts (KCl, NaCl, Na₂HPO₄, NaH₂PO₄) were purchased from Reachim (Russia). Ion-selective membrane components high molecular weight poly(vinylchloride) (PVC), 2-nitrophenyl octyl ether (o-NPOE) were obtained from Fluka. Potassium tetrakis(4-chlorophenyl)borate (KTCIPB) were purchased from Merck. FeCl₃·6H₂O, K₃[Fe(CN)₆], ionophore valinomycin, tetrahydrofuran (THF) were obtained from Sigma Aldrich (Germany). THF was distilled before use.

Planar screen-printed three-electrode structures with carbon working electrode ($\varnothing = 1.8$ mm) and Ag-reference electrode produced by Ltd. Rusens (Russia) were used for electrochemical investigations.

2.2. Instrumentation

Electrochemical measurements were carried out with μ AUTOLAB III (Metrohm, The Netherlands). Electrochemical impedance spectra (EIS) were recorded using a PalmSens 4 (PalmSens, Netherlands). The flow injection setup included a Perfusor Compact S syringe pump (Braun, Germany), injector (IDEX Health & Science LLC) and plexiglass wall-jet cell with a 0.5 mm nozzle (Rusens, Russia).

2.3. Methods

2.3.1. Modification of the screen-printed electrodes with Prussian blue.

Screen printed electrodes (SPE) were modified either by electrochemically synthesized PB films or by catalytically synthesized PB nanoparticles. Electrodeposition of PB film on SPE was performed from a solution containing 4 mM FeCl₃ and K₃[Fe(CN)₆] in 0.1 M KCl/HCl via cyclic voltammetry. The potential was cycled from 0.75 to 0.4 V at sweep rate of 40 mV·s⁻¹ during 2-6 cycles.

Catalytic synthesis of PB nanoparticles was carried out as reported previously [12]. In brief, hydrogen peroxide was added to equimolar mixture of FeCl₃ and K₃[Fe(CN)₆] (50 mM) in 0.1 M KCl/HCl upon ultrasonication. After centrifugation, the resulting nanoparticles were redispersed 5-7 times into 0.1 M KCl/HCl solution. For SPE modification 2 μ l of PB nanoparticles (0.1–0.5 mM) was drop-cast onto surface of working electrode. After modification the electrodes were annealed at 100°C for 1 hour.

The amount of PB on the modified electrodes was controlled electrochemically from the peak area on cyclic voltammogram in the supporting electrolyte (0.1 M KCl/HCl). The amount of the electroactive PB was 5–20 nmol/cm².

The analytical characteristics of the obtained sensors were compared in the flow-injection mode at a fixed potential, recording the current generated by sensor upon the injection of a salt solution (KCl or NaCl) of a known concentration. The flow rate was 40.2 ml·h⁻¹.

2.3.2. Solid contact ISE preparation

Membrane cocktail was prepared by mixing 32 wt% PVC, 63.5 wt% o-NPOE, 0.5 wt% potassium tetrakis(4-chlorophenyl)borate (KTpCIPB) and 4 wt% ionophore (valinomycin). 100 mg of membrane components were dissolved in various amount of THF (0.5, 0.66, 0.75, 1, 1.25 and 1.5 ml). The membrane cocktail density was estimated as the ratio of the mass of the ISM components to the volume of added THF. Then membrane cocktail was spin-coated onto electrodes modified with PB nanoparticles by casting

3 μl of the cocktail at 1000 rpm. The sensors were conditioned in aqueous 0.1 M KCl at least 12 hours before measurements.

EIS spectra were recorded at E_{dc} 0.1 V, from 50 kHz to 1 Hz in 0.1 M KCl/HCl.

3. Results and discussion

The elaborated SC-ISE involves the PB nanoparticles as a solid contact. Modification of the electrode surface with PB nanoparticles was performed simply and not time-consuming in contrast to electrochemical PB synthesis. Suspension containing catalytically synthesized PB nanoparticles was drop-cast on the surface of the working electrode and annealed after drying. Before the coating with ion-selective membrane (ISM), the intrinsic selectivity of PB for potassium ions was investigated. PB nanoparticles-modified sensors without PVC membrane were studied in the flow-injection amperometry mode under constant potential. Upon injection of potassium chloride solutions PB generates a current response as a couple of oppositely directed peaks: after the major sharp cathodic peak, a smaller anodic peak is observed (Figure 1a). The peak current increase with increasing the concentration of potassium chloride. Previously for SC-ISE based on conductive polymers (polyaniline, PEDOT) it was shown that the first peak is the analytical signal [4,5]. Hence, the sensor sensitivity was estimated from the plot of the cathodic current peak versus the concentration of potassium chloride. In this system the appearance of the cathodic peak is associated with the reduction of PB to Prussian white, this process is accompanied by cation intercalation for charge compensation [13]. Therefore, it is necessary to select the optimal potential used for amperometry. Figure 1b shows that the maximum sensitivity of the sensors is achieved at a potential 0.1 V, when the PB exists in the fully reduced form.

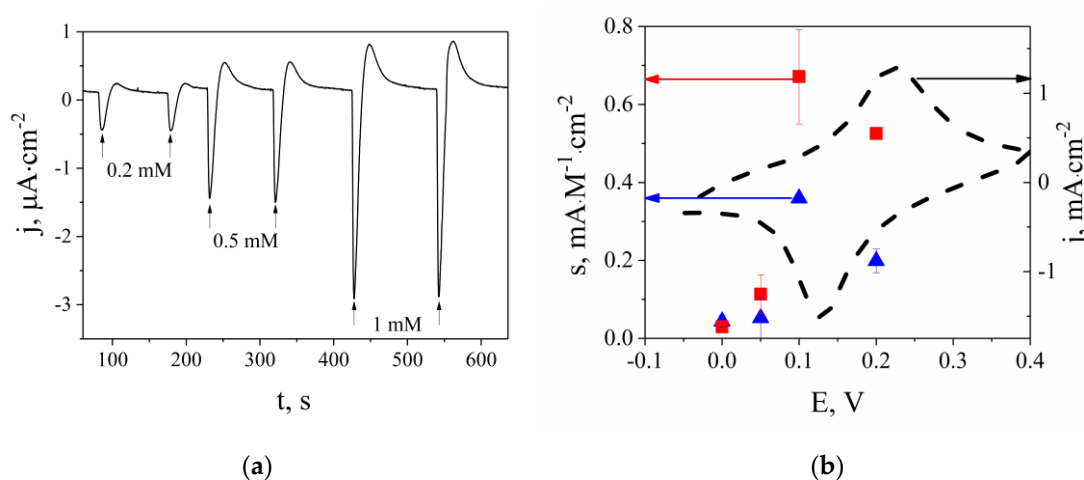


Figure 1. (a) Flow-injection amperometry of KCl solutions in 0.1 M HCl using PB nanoparticles- modified screen-printed electrodes without ion-selective membrane, $E_{dc} = 0.1$ V. (b) The dependence of the sensitivity of PB nanoparticles modified electrodes on the potential in the amperometric determination of potassium (■) and sodium (▲) ions (0.1 M HCl); corresponding sensor cyclic voltammogram (0.1 M KCl/HCl; 40 mV/s).

Since the PB nanoparticles are not covered by an ISM, the injection of a sodium chloride solution also results in a cathodic peak, but the sensitivity to sodium cations is lower than to potassium by a factor of 4. Therefore, the intrinsic selectivity of Prussian Blue was observed. These sensors were compared with electrodes modified electrochemically with PB films. The sensors based on PB nanoparticles demonstrated a six-fold increase in sensitivity (up to 0.7 ± 0.1 $\text{mA} \cdot \text{M}^{-1} \cdot \text{cm}^{-2}$) compared to the sensors based on PB films with a similar amount of electroactive PB. Thus, PB nanoparticles are the suitable material for SC-ISE elaboration.

In order to improve selectivity, the ISMs of different compositions were deposited by spin-coating on the working electrode with adsorbed PB nanoparticles. With an in-

crease in the amount of THF, the density of the membrane cocktail decreases. It was assumed that denser membranes improve the stability of the sensor, but simultaneously prevent a noticeable decrease in sensitivity. Charge transfer also depends on the amount of PB, but it was the same for the compared sensors.

The effect of film thickness on the charge transfer resistance was investigated using EIS. In Nyquist plots, the EIS spectrum shows a semicircle in the high frequency region (Figure 2a). The diameter of the semicircle depends on E_{dc} reaching a minimum at 0.1 V. With an increasing ISM density, the diameter of the semicircle in spectra of the sensors also increases (Figure 2b). It was found out that the sensitivity of sensors increases in the flow-injection detection of potassium ions with decrease of charge transfer resistance. As a result, the maximum sensitivity is achieved by diluting 100 mg of the membrane cocktail in 1.5 mL of THF.

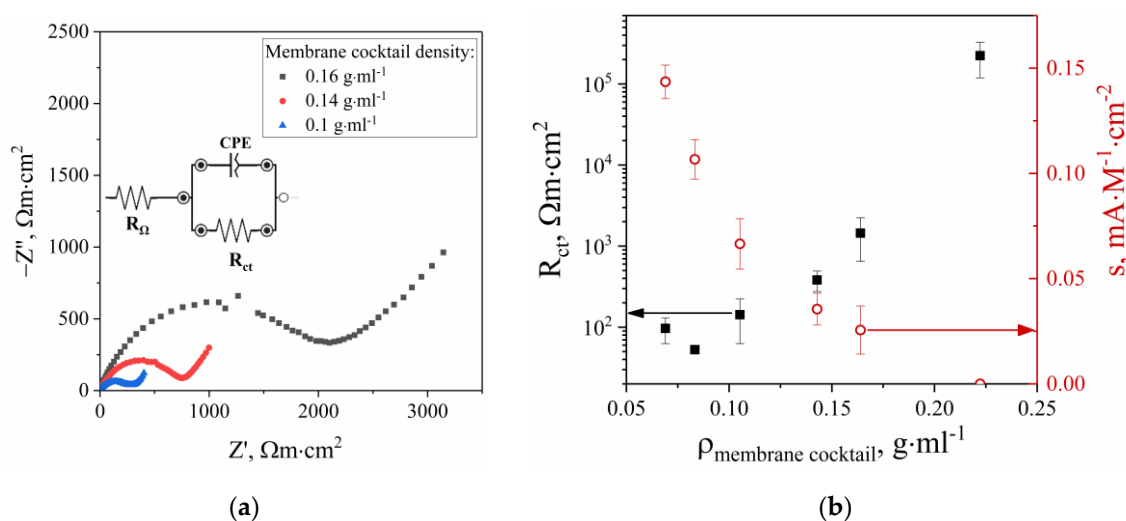


Figure 2. (a) Nyquist plots from EIS of sensors based on PB nanoparticles coated on ISM with various composition. Inset: the equivalent circuit used in the fitting. ($E_{dc}=0.1$ V; 0.1 M KCl/HCl). (b) Dependence of the charge transfer resistance (■) and the sensitivity of the sensors (●) on the ion-selective membrane cocktail density.

For the analysis of biological fluids, it is preferable that measurements are taken in buffer solution, rather than HCl. However, due to the possibility of interfering cations intercalation (especially NH_4^+ , Na^+ , Ca^{2+} , Mg^{2+}), it is difficult to select a buffer for FIA. For example, if sodium phosphate buffer is used as a carrier (pH 6.0), an excess of interfering sodium ions is constantly present in the solution. In this case the selectivity of the sensor is reduced by a factor of 20, compared with the selectivity in 0.1 M hydrochloric acid. In order to improve selectivity, it is preferable to carry out measurements in a buffer solution without interfering ions.

To eliminate the interfering effect of cations in the supporting electrolyte we proposed to use the Bis-Tris buffer. In Bis-Tris sensors based on PB nanoparticles without a ISM demonstrate intrinsic selectivity for potassium ions: the response to sodium is two times lower.

To improve the selectivity ISM membrane was spin-coated. As it was discussed earlier the sensor sensitivity depends on potential used for amperometry, and maximum sensitivity is achieved for Prussian White at -0.1 V. Therefore, the dependence on the concentration of potassium chloride in the FIA mode was recorded at this potential. The current response is linearly dependent on the concentration of potassium chloride in the range from $2.5 \cdot 10^{-5}$ to $1 \cdot 10^{-3}$ M (Figure 3). As a result of coating the PB nanoparticles with ISM, the sensitivity in Bis-Tris became equal to 3.6 ± 0.4 $\text{mA} \cdot \text{M}^{-1} \cdot \text{cm}^{-2}$, which is comparable to a sensor based on PEDOT(PSS) [5]. Separate solution method was used to find the selectivity coefficient $\log K_{\text{Na}^+/\text{K}^+} = -2.7$. Therefore, the absence of sodium ions in buffer increases the selectivity of the sensors by almost 100 times.

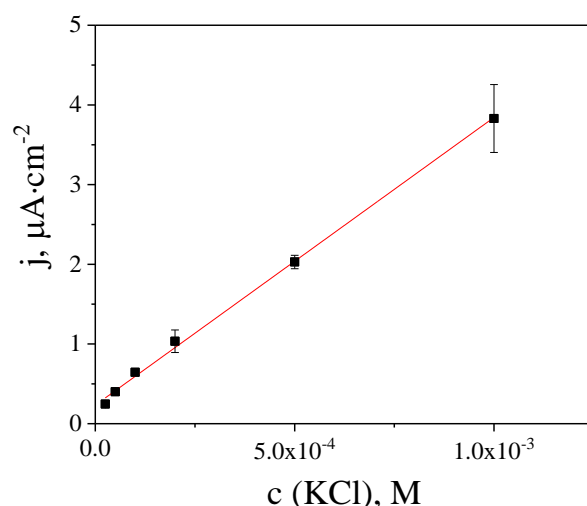


Figure 3. Calibration plot in flow-injection amperometric mode for PB nanoparticles modified electrode covered with K⁺-selective membrane (E=-0.1 V; 50 mM Bis-Tris, pH 6.0).

To sum up, the proposed sensors in combination with flow-injection amperometric mode provides the fast and selective analysis applicable for biological fluids. The elaborated SC-ISE are easy to produce, and their response time does not exceed 40 seconds in flow-injection system. Since in the blood serum the concentration of sodium is 20-40 times higher than potassium, the achieved selectivity is sufficient and biological objects can be examined using the sensor.

Author Contributions: V.S. — investigation, visualization, original draft preparation; V.N. — conceptualization, methodology, review and editing; A.K. — supervision, conceptualization, methodology. All authors have read and agreed to the published version of the manuscript.

Funding: This research was funded by the Russian Science Foundation, grant number 19-13- 00131 (<https://rscf.ru/en/project/19-13-00131/>).

Institutional Review Board Statement: Not applicable.

Informed Consent Statement: Not applicable.

Conflicts of Interest: Not applicable.

References

1. Tseng, C.-C.; Lu, S.-Y.; Chen, S.-J.; Wang, J.-M.; Fu, L.-M.; Wu, Y.-H. Microfluidic Aptasensor POC Device for Determination of Whole Blood Potassium. *Anal. Chim. Acta* **2022**, *1203*, 339722, doi:10.1016/j.aca.2022.339722.
2. Bondar, A. V.; Keresten, V.M.; Mikhelson, K.N. Ionophore-Based Ion-Selective Electrodes in Non-Zero Current Modes: Mechanistic Studies and the Possibilities of the Analytical Application. *J. Anal. Chem.* **2022**, *77*, 145–154, doi:10.1134/S1061934822020046/FIGURES/3.
3. Kałuża, D.; Michalska, A.; Maksymiuk, K. Solid-Contact Ion-Selective Electrodes Paving the Way for Improved Non-Zero Current Sensors: A Minireview. *ChemElectroChem* **2022**, *9*, doi:10.1002/celec.202100892.
4. Zavolskova, M.D.; Nikitina, V.N.; Maksimova, E.D.; Karyakina, E.E.; Karyakin, A.A. Constant Potential Amperometric Flow-Injection Analysis of Ions and Neutral Molecules Transduced by Electroactive (Conductive) Polymers. *Anal. Chem.* **2019**, *91*, 7495–7499, doi:10.1021/acs.analchem.9b00934.
5. Nikitina, V.N.; Maksimova, E.D.; Zavolskova, M.D.; Karyakin, A.A. Flow Injection Amperometry as an Alternative to Potentiometry for Solid Contact Ion-Selective Membrane-Based Electrodes. *Electrochim. Acta* **2021**, *377*, 138074, doi:10.1016/j.electacta.2021.138074.
6. Shao, Y.; Ying, Y.; Ping, J. Recent Advances in Solid-Contact Ion-Selective Electrodes: Functional Materials, Transduction Mechanisms, and Development Trends. *Chem. Soc. Rev.* **2020**, *49*, 4405–4465, doi:10.1039/C9CS00587K.
7. Itaya, K.; Uchida, I.; Neff, V.D. Electrochemistry of Polynuclear Transition Metal Cyanides: Prussian Blue and Its Analogues. *Acc. Chem. Res.* **1986**, *19*, 162–168, doi:10.1021/AR00126A001/ASSET/AR00126A001.FP.PNG_V03.
8. Krishnan, V.; Xidis, A.L.; Neff, V.D. Prussian Blue Solid-State Films and Membranes as Potassium Ion-Selective Electrodes. *Anal. Chim. Acta* **1990**, *239*, 7–12, doi:10.1016/S0003-2670(00)83828-3.

9. Ghosh, T.; Chung, H.-J.; Rieger, J. All-Solid-State Sodium-Selective Electrode with a Solid Contact of Chitosan/Prussian Blue Nanocomposite. *Sensors* **2017**, *17*, 2536, doi:10.3390/s17112536.
10. Ang, J.Q.; Nguyen, B.T.T.; Toh, C.S. A Dual K⁺-Na⁺ Selective Prussian Blue Nanotubes Sensor. *Sensors Actuators B Chem.* **2011**, *157*, 417–423, doi:10.1016/J.SNB.2011.04.076.
11. Gabrielli, C.; Hémerly, P.; Liatsi, P.; Masure, M.; Perrot, H. An Electrogravimetric Study of an All-Solid-State Potassium Selective Electrode with Prussian Blue as the Electroactive Solid Internal Contact. *J. Electrochem. Soc.* **2005**, *152*, H219, doi:10.1149/1.2104047.
12. Komkova, M.A.; Karyakina, E.E.; Karyakin, A.A. Catalytically Synthesized Prussian Blue Nanoparticles Defeating Natural Enzyme Peroxidase. *J. Am. Chem. Soc.* **2018**, *140*, 11302–11307, doi:10.1021/jacs.8b05223.
13. Itaya, K.; Ataka, T.; Toshima, S. Spectroelectrochemistry and Electrochemical Preparation Method of Prussian Blue Modified Electrodes. *J. Am. Chem. Soc.* **1982**, *104*, 4767–4772, doi:10.1021/ja00382a006.