

PEDOT-based Chemiresistive and Colorimetric Dual-Mode Sensors for the Detection of Hydrogen Peroxide Vapor

Siyang An ¹, Xiaowen Xie ¹, Nan Gao ¹, Shuai Chen ^{1,2,*}¹ School of Pharmacy, Jiangxi Science & Technology Normal University, Nanchang, Jiangxi, 330013, China;² Jiangxi Provincial Engineering Research Center for Waterborne Coatings, Nanchang, Jiangxi, 330013, China.

* Correspondence: shuaichen@jxstnu.edu.cn (S.C.); Tel.: +86-791-83832345 (S.C.).

Abstract: Hydrogen peroxide (H₂O₂) is widely used aqueous solution for oxidation, disinfection and sterilization, and its detection is very important in the fields of biological health and environment. The main detection methods of H₂O₂ include colorimetric, electrochemical, enzymatic and fluorescence analysis. However, due to the influence of moisture and oxidation, it is very scarce to realize the simple, convenient, real-time and efficient detection technology for hydrogen peroxide vapor (HPV). Recently, our group proposed to add ammonium titanyl oxalate (ATO) to the sensing film composite system to prepare a chemosensor based on PEDOT:PSS-ATO/PEDOT composite film, the limit of detection (LOD) of the film is 1.0 ppm, and the linear trend is in the range of 1.0 ppm to 10.5 ppm. and explored the influence of various material systems on its HPV sensing performance both giving electrical and colorimetric response. This study was expected to realize a practical HPV sensor as well as promote the further application of PEDOT-based composites in the field of chemosensors.

Keywords: PEDOT:PSS; hydrogen peroxide; gas detection; chemiresistive; colorimetric

1. Introduction

Hydrogen peroxide (H₂O₂) aqueous solution is an environmentally friendly and efficient oxidant and disinfectant. The outbreak of the novel coronavirus has led to the strengthening of disinfection and sterilization measures in public facilities, transportation, hospitals, nursing homes, and even ordinary families all over the world [1,2]. However, its wide use has brought some hazards. For example, the strong oxidative properties of H₂O₂ may cause corrosion and irritation to the skin, eyes and mucous membranes of the human body. If it enters the human body, oxidative stress reactions may occur to generate free radicals, resulting in cell damage and some diseases, and accelerating the growth of the human body. Therefore, in view of the importance of biological and environmental safety, it is very important to develop effective detection technologies for H₂O₂.

At present, most of the research on H₂O₂ sensors focused on its detection in liquid phase systems [3]. In view of its wide use as environmental disinfectants and explosive markers, the importance of H₂O₂ vapor (HPV) monitoring in the air also cannot be ignored. In most cases, the HPV detection is by firstly making it cool and adsorption in water, and then using electrochemical methods to measure the liquid concentration [4]. In addition, the detection of HPV can also be achieved by fluorescence analysis [5,6], colorimetry [7], etc. Fluorescence methods generally have high sensitivity and selectivity, but there is a problem of cumbersome material synthesis. In comparison, the colorimetric method is simple, fast and direct, and is seen as an important direction for sensor popularization research. On the other hand, the chemiresistive sensor is often used to monitor humidity and various gases, and has the advantages of low cost, small size, easy to use, facile to construct device and real-time monitoring.

Citation: To be added by editorial staff during production.

Academic Editor: Firstname Last-name

Published: date

Publisher's Note: MDPI stays neutral with regard to jurisdictional claims in published maps and institutional affiliations.



Copyright: © 2022 by the authors. Submitted for possible open access publication under the terms and conditions of the Creative Commons Attribution (CC BY) license (<https://creativecommons.org/licenses/by/4.0/>).

To explore effective HPV sensing materials, recently, our group investigated the applicability of poly(3,4-ethylenedioxythiophene) (PEDOT)-based chemiresistive and colorimetric dual-mode sensors [8,9]. Among them, poly(3,4-ethylenedioxythiophene):polystyrene sulfonate (PEDOT:PSS)-ammonium titanyl oxalate (ATO)/PEDOT composite film was demonstrated as a good platform for high selective, sensitive and naked-eye HPV sensing. The system was designed for the following reasons [5].

On one hand, intrinsically conductive polymers (ICPs), especially PEDOT family, are considered to be an important and good candidate sensing materials [10]. Their unique tunable electrical properties, as well as the advantages of easy synthesis, structural diversity, functionalization, and flexibility make them versatile in sensor applications. At present, the application of PEDOT in this field has developed into many types such as electrochemistry, chemoresistance, piezoelectricity, etc. In particular, their unique doping/dedoping process makes them one of the most promising candidates for chemistoric sensor applications for gas detection at room temperature [11]. Among this aspect, PEDOT:PSS has special advantages [12], and has also been studied on electrochemical detection of H_2O_2 in liquid phase system, and chemistoric response to many gas phase analytes like NH_3 , CO , NO_x , etc.

On the other hand, the hygroscopicity of PEDOT:PSS film itself is conducive to the adsorption of HPV, and the electrical and optical properties will be affected by the oxidation of HPV. And, hydrophobic PEDOT outer layer could improve the film surface roughness and weaken its hygroscopicity, which will help maintain its stability and sensing accuracy especially under high humidity.

Moreover, in view of the fact that, HPV is difficult to distinguish by smell and vision due to its colorless and light-odor, ATO, as a colorless compound but has characteristic complexation-induced discoloration with H_2O_2 , was introduced into the gas-sensitive material system. It can basically eliminate the interference of all coexisting gases in the normal environment and thus ensure the high selectivity [5]. At the same time, the color change reaction will provide a colorimetric sensing signal, which enhances the signal readability.

2. Materials and Methods

In this work, spin-coating the PEDOT:PSS/ATO dispersion on the ITO conducting glass and dried in an oven at $50\text{ }^\circ\text{C}$ to prepared PEDOT:PSS-ATO film. The electrochemical correlation tests were performed using a three-electrode system. The well-prepared PEDOT:PSS-ATO film was selected as the working electrode, the platinum sheet as the counter electrode, Ag/AgCl as the reference electrode, acetonitrile/tetrabutylammonium hexafluorophosphate (0.1 M) as the electrolyte and EDOT (1 mM) was added in as a unit of electropolymerization. The PEDOT layer with a certain amount of polymerization charge was electrodeposited on the surface of the composite film by electrochemical polymerization, and the PEDOT:PSS-ATO/PEDOT composite film was prepared. After that, we explored the resistance response and colorimetric response behavior and effect of the composite film under different concentrations of HPV.

3. Results and Discussion

The PEDOT:PSS-ATO and PEDOT:PSS-ATO/PEDOT composite films were prepared by conventional mechanical blending and electrochemical methods [7,8].

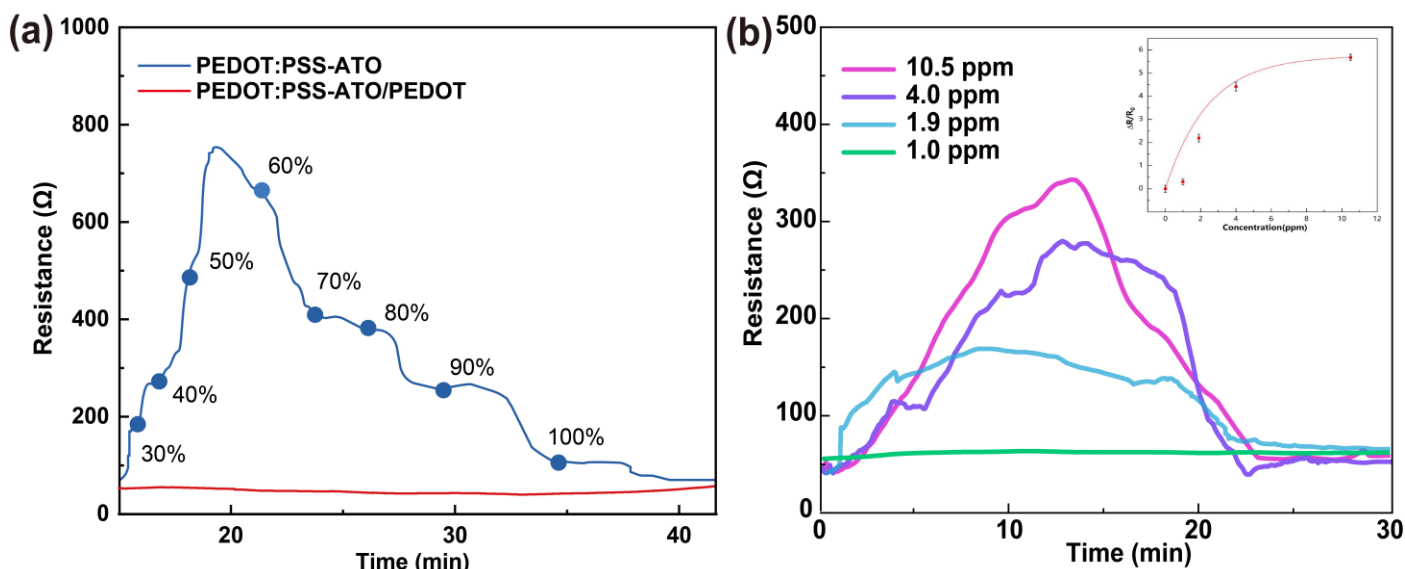


Figure 1. (a) PEDOT:PSS-ATO and PEDOT:PSS-ATO/PEDOT films under increasing levels of ambient humidity (30~100% RH); (b) Resistance-time curve of PEDOT:PSS-ATO/PEDOT film (Inset: resistance response-HPV concentration fitting curve of PEDOT:PSS-ATO/PEDOT film).

As seen in **Figure 1a**, the PEDOT:PSS-ATO film exhibited a typical moisture response of PEDOT:PSS film. As the humidity increases, the resistance value reaches the maximum value (about 20 min, 7.6 times of the initial value) at about 50%~60% RH. And then with the increases of the humidity, the resistance of film was continued to decrease until fell to the same level as the initial value. The resistance response curve (**Figure 1b**) of the PEDOT:PSS-ATO/PEDOT composite film was similar to that of the PEDOT:PSS/PEDOT film [8]. The resistance of the PEDOT:PSS-ATO/PEDOT film increased rapidly from the initial value (about 53 Ω, the PEDOT:PSS/PEDOT film was about 48 Ω) and decreased rapidly until reaching similar levels to their initial values after 20 min. The resistance response values ($\Delta R/R_0$) calculated by the peak value are 5.68 (10.5 ppm), 4.42 (4.0 ppm), 2.19 (1.9 ppm), 0.30 (1.0 ppm), respectively, and the time to reach the peak value is 14 min, 13 min, 9 min, and 10 min. Compared with our previous reported, the reaction of ATO with H_2O_2 consumes part of HPV while generating the H_2O , thus speeding up the entire process of HPV film detection. Under the coverage of the PEDOT layer, the H_2O generated by reaction of ATO and H_2O_2 was locked in the PEDOT:PSS-ATO layer, which accelerated the detection process. All samples were tested in parallel three times and taken their average values. The resistance response-HPV concentration data of the PEDOT:PSS-ATO/PEDOT composite film was fitted using the ExpAssoc function, the final fitting curve is shown in **Figure 1b** (inset), $y = 5.75634 \times (1 - e^{-(x/2.42891)})$, $R^2 = 0.85399$.

Here we evaluate the colorimetric sensing by the ΔE value. ΔE is the comprehensive total color difference, which can be calculated by the formula:

$$\Delta E = [(\Delta L)^2 + (\Delta a)^2 + (\Delta b)^2]^{1/2} \quad (1)$$

Where ΔL , Δa , Δb are the effects of PEDOT-based composite film on HPV. The colorimetric signal response to the color difference test results can be tested and recorded by a portable color difference meter [9]. According to the results shown in **Figure 2**, the ΔE value [9] of PEDOT:PSS film increased with the increase of HPV concentration, even at low concentrations (1.0 ppm), a relative slightly color difference can be observed with the naked eye ($\Delta E = 2.11$). However, when PEDOT was deposited on the PEDOT:PSS film, with the increase of HPV concentration, the color change after the detection of HPV by the composite film was not obvious, and only when the original composite film was compared with the composite film that had detected HPV concentrations of 10.5 ppm, the naked eye could slightly detect the color change ($\Delta E = 2.08$). The PEDOT layer on the surface can not only slow down the immersion of moisture, but also hinder the entry of

H₂O₂ components, which weakens the colorimetric response generated by the interaction between PEDOT:PSS layer and H₂O₂ components to a certain extent. The oxidative color-changing substance ATO, which characteristic responded to H₂O₂, was added to the PEDOT:PSS aqueous dispersion by mechanical blending, and PEDOT:PSS-ATO and PEDOT:PSS-ATO/PEDOT composite films were prepared. With the introduction of HPV and the increase of the concentration, the two composite films were observed to change from blue to yellow-green. Since ATO can react with H₂O₂ in a highly selective color change, compared with the monotonous blue shades of PEDOT:PSS and PEDOT, the detection of HPV by PEDOT:PSS-ATO and PEDOT:PSS-ATO/PEDOT composite films presents a richer and more obvious color change signal, so that the naked eye can more clearly identify the working condition of the sensor, and at 1.0 ppm concentration of HPV, the ΔE value of PEDOT:PSS-ATO composite films reached 2.6. In 4.0 ppm and 10.5 ppm concentration of HPV, the film color was obviously yellowish green. Compared with the colorimetric response of HPV detected by PEDOT:PSS/PEDOT composite film, the ΔE values of PEDOT:PSS-ATO/PEDOT composite films are higher. When the concentration of HPV is 1.0 ppm, the color change of the film can be slightly detected ($\Delta E= 1.57$). Colorimetric response increased by nearly 128% at the same concentration, and the color change under naked eye was more significant.

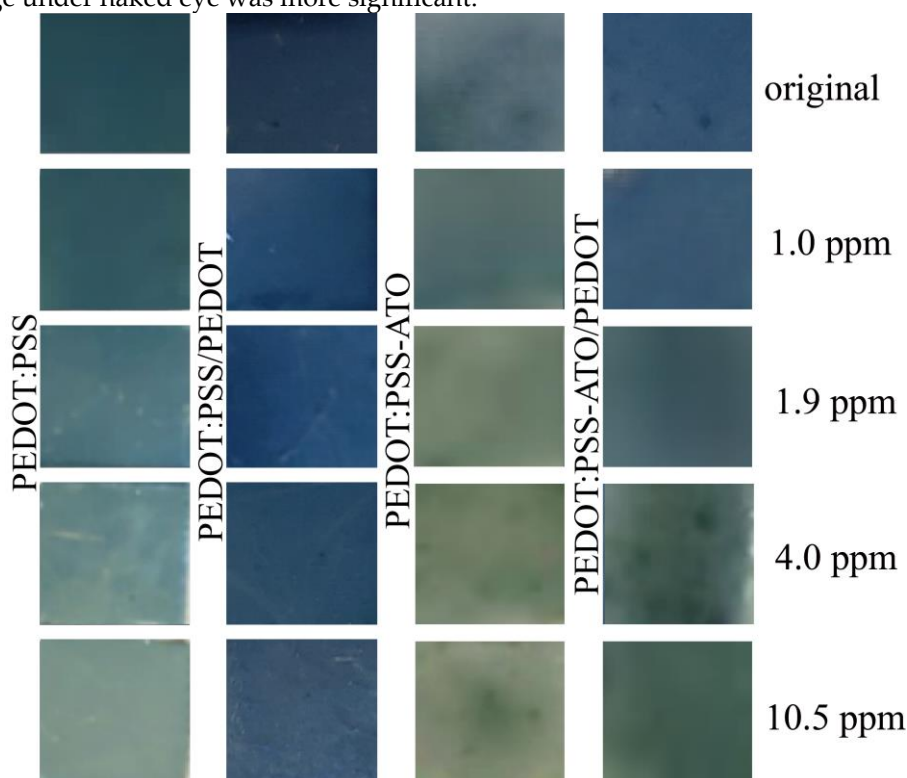


Figure 2. Photos of PEDOT, PEDOT:PSS, PEDOT:PSS-ATO and PEDOT:PSS-ATO/PEDOT films before and after testing of different concentrations of HPV.

Table 1. Comparison of detection linear range and detection limit of sensors for hydrogen peroxide vapor detection.

Electrode Materials	Linear Range [ppm]	LOD [ppm]	References
PEDOT:PSS-ATO/PEDOT	1.0~10.5	1.0	This work
Paper-based ofibril materials	N/A	4.3	[5]

Titanium(IV)-based peroxide detection test strips	2.0~30.0	1.0	[13]
--	----------	-----	------

The paper-based colorimetric sensing system [5] published in 2011 by Prof. Zang Ling's research group, which has made breakthrough contributions to HPV detection. It can detect hydrogen peroxide vapor exceeding a few parts per billion, with a detection limit of 4.3 ppm. Titanium-based peroxide test paper [13], during exposure to peroxide vapor in the peroxide concentration range from 2.0 to 30.0 ppm, first-order behavior of color change with time was observed, and the detection limit was also as low as 1.0 ppm. Comparing the linear range and limit of determination (LOD) with other sensors for hydrogen peroxide detection (Table 1), it can be seen that the PEDOT:PSS-ATO/PEDOT film sensor has a lower detection limit and can achieve low-concentration target analysis object detection. Different from liquid phase detection, research on HPV detection is lacking. Our work not only studies the effect of applying PEDOT:PSS-based gas-sensing materials to HPV varistor sensing, but also enhances the effect of colorimetric signal detection. The future optimization of the PEDOT:PSS-based composite system using the dual-mode detection mechanism provides theoretical support.

4. Conclusions

In summary, ATO was added to the PEDOT:PSS aqueous dispersion to prepare PEDOT:PSS-ATO film and then EDOT was electrochemically polymerized at its surface forming PEDOT:PSS-ATO/PEDOT composite film. It was successfully used for chemiresistive and colorimetric detection of HPV. Since ATO can react with H₂O₂ in a highly selective color change, compared with the monotonous blue shade change of PEDOT:PSS and PEDOT films, the detection of HPV by these films showed a much richer and more pronounced color change signal allowing the naked-eye identification. Especially, PEDOT:PSS-ATO/PEDOT film can detect HPV at a low concentration of 1.0 ppm via dual modes, which provides its application prospect for practical HPV monitoring under the safety threshold.

Author Contributions: Conceptualization, S.C.; methodology, S.C. and N.G.; software, S.A., N.G. and X.X.; validation, X.X. and N.G.; formal analysis, S.A.; investigation, N.G. and S. C.; resources, S.C.; data curation, N.G.; writing—original draft preparation, S.A. N.G. and X.X.; writing—review and editing, S.C.; supervision, S.C.; project administration, S.C.; funding acquisition, S.C.

Funding: This work was funded by the Academic Development Project of TongXin Funds (grant number 2023161808).

Institutional Review Board Statement: Not applicable.

Informed Consent Statement: Not applicable.

Data Availability Statement: Not applicable.

Conflicts of Interest: The authors declare no conflict of interest.

References

- Berger, D.; Gundermann, G.; Sinha, A.; Moroi, M.; Goyal, N.; Tsai, A. Review of aerosolized hydrogen peroxide, vaporized hydrogen peroxide, and hydrogen peroxide gas plasma in the decontamination of filtering facepiece respirators. *Am. J. Infect. Control*, **2022**, *50*, 203–213.
- Dewey, H.M.; Jones, J.M.; Keating, M.R.; Budhathoki-Uprety, J. Increased use of disinfectants during the COVID-19 pandemic and its potential impacts on health and safety. *ACS Chem. Health Saf.*, **2022**, *29*, 27–38.
- Pashkova, A.; Svajda, K.; Black, G.; Dittmeyer, R. Automated system for spectrophotometric detection of liquid phase hydrogen peroxide for concentrations up to 5% w/w. *Rev. Sci. Instrum.*, **2009**, *80*, 055104.
- Zhao, F.J.; Zhou, S.; Zhang, Y.J. Ultrasensitive detection of hydrogen peroxide using Bi₂Te₃ electrochemical sensors. *ACS Appl. Mater. Interfaces*, **2021**, *13*, 4761–4767.
- Xu, M.; Bunes, B.R.; Zang, L. Paper-based vapor detection of hydrogen peroxide: Colorimetric sensing with tunable interface. *ACS Appl. Mater. Interfaces*, **2011**, *3*, 642–647.

6. Zhang, Y.M.; Feng, Y.T.; Zhang, Z.X.; Zhang, M. Highly efficient fluorescent film probe of hydrogen peroxide vapor. *Microchem. J.*, **2020**, *158*, 105290.
7. Tran, H.V.; Nguyen, T.V.; Nguyen, L.T.N.; Hoang, H.S.; Huynh, C.D. Silver nanoparticles as a bifunctional probe for label-free and reagentless colorimetric hydrogen peroxide chemosensor and cholesterol biosensor. *J. Sci. Adv. Mater. Devices*, **2020**, *5*, 385–391.
8. Xie, X.W.; Gao, N.; Zhu, L.; Hunter, M.; Chen, S.; Zang, L. PEDOT:PSS/PEDOT film chemiresistive sensors for hydrogen peroxide vapor detection under ambient conditions. *Chemosensors*, **2023**, *11*, 124.
9. Xie, X.W.; Gao, N.; Hunter, M.; Zhu, L.; Yang, X.M.; Chen, S.; Zang, L. PEDOT films doped with titanyl oxalate as chemiresistive and colorimetric dual-mode sensors for the detection of hydrogen peroxide vapor. *Sensors*, **2023**, *23*, 3120.
10. Ali M.Z.; Ishak, K.M.K.; Zawawi, M.A.M.; Zulkifli, Z.; Jaafar, M.; Ahmad, Z. Single-step treatment to improve conductivity of PEDOT:PSS by hydrobromic acid solution for application of transparent electrode. *Org. Electron.*, **2022**, *110*, 106643.
11. Gao, N.; Yu, J.R.; Tian Q.Y.; Shi, J.F.; Zhang, M.; Chen, S.; Zang, L. Application of PEDOT:PSS and its composites in electrochemical and electronic chemosensors. *Chemosensors*, **2021**, *9*, 79.
12. Vigna, L.; Verna, A.; Marasso, S. L.; Sangermano, M.; D'Angelo, P.; Pirri, F. C.; Cocuzza, M. The effects of secondary doping on ink-jet printed PEDOT:PSS gas sensors for VOCs and NO₂ detection. *Sens. Actuators B Chem.*, **2021**, *345*, 130381.
13. Hossain, R.; Dickinson, J.J.; Apblett, A.; Materer, N.F. Detection of Hydrogen Peroxide in Liquid and Vapors Using Titanium(IV)-Based Test Strips and Low-Cost Hardware. *Sensors*, **2022**, *22*, 6635.