

Proceeding Paper

Microfabricated Gold Aptasensors for the Label-Free Electrochemical Assay of Oxytetracycline Residues in Milk [†]

Vassilis Machairas ¹, Andreas Anagnostopoulos ¹, Dionysios Soulis ¹, Anastasios Economou ^{1,*}, Kristóf Jakab ², Nikitas Melios ^{1,3}, Zsófia Keresztes ², George Tsekis ³, Joseph Wang ⁴ and Thanassis Speliotis ⁵

¹ Department of Chemistry, National and Kapodistrian University of Athens, 157 71 Athens, Greece; vasilismax42@gmail.com (V.M.); adreasanagno@gmail.com (A.A.); dsoulis1@gmail.com (D.S.); nmelios@bioacademy.gr (N.M.)

² Research Centre for Natural Sciences, Institute of Materials and Environmental Chemistry, Functional Interfaces Research Group, Magyar tudósok krt. 2., 1117 Budapest, Hungary; jakab.kristof@ttk.hu (K.J.); keresztes.zsofia@ttk.hu (Z.K.)

³ Biomedical Research Foundation, Academy of Athens, 4 Soranou Ephessiou Street, 115 27 Athens, Greece; gtsekis@bioacademy.gr

⁴ Department of Nanoengineering, University California San Diego (UCSD), La Jolla, CA 92093-0448, USA; josephwang@ucsd.edu

⁵ Institute of Nanoscience and Nanotechnology, NCSR “Demokritos”, Aghia Paraskevi, 15310 Athens, Greece; t.speliotis@inn.demokritos.gr

* Correspondence: aeconomou@chem.uoa.gr; Tel.: +30-210-7274298

[†] Presented at the 10th International Electronic Conference on Sensors and Applications (ECSA-10), 15–30 November 2023; Available online: <https://ecsa-10.sciforum.net/>.

Abstract: In this work, we describe a new type of electrochemical aptasensor for the label-free detection of oxytetracycline (OTC). Thin-film gold electrodes were fabricated by sputtering gold on a Kapton film, followed by the immobilization of a thiol-modified aptamer on the electrode surface. Selective capture of OTC at the aptamer-functionalized electrodes was monitored electrochemically with the use of the Fe(CN)₆⁴⁻/Fe(CN)₆³⁻ redox probe. Different experimental variables were studied through which the metrological features for OTC determination were derived. Finally, the developed sensor was implemented towards the detection of OTC in a spiked milk sample.

Keywords: aptasensor; electrochemical; oxytetracycline; label-free; microfabrication; gold electrodes

Citation: Machairas, V.; Anagnostopoulos, A.; Soulis, D.; Economou, A.; Jakab, K.; Melios, N.; Keresztes, Z.; Tsekis, G.; Wang, J.; Speliotis, T. Microfabricated Gold Aptasensors for the Label-Free Electrochemical Assay of Oxytetracycline Residues in Milk. *Eng. Proc.* **2023**, *56*, x. <https://doi.org/10.3390/xxxxx>

Academic Editor(s): Name

Published: 15 November 2023



Copyright: © 2023 by the authors. Submitted for possible open access publication under the terms and conditions of the Creative Commons Attribution (CC BY) license (<https://creativecommons.org/licenses/by/4.0/>).

1. Introduction

Oxytetracycline (OTC) is a commonly-used antibiotic in veterinary medicine; residues of OTC can be present in animal-derived food and are therefore, consumed by humans [1]. The consumption of, and long-term exposure to, antibiotics may induce antibiotic resistance and can be harmful to human health [2], therefore maximum residue limits (MRLs) in foodstuff of animal origin have been set by the European Union for antibiotics [3]; in particular, an MRL of 100 µg L⁻¹ for OTC residues in milk has been established.

Therefore, it is essential to develop methods for the sensitive and specific detection of OTC in the environment and food products [4]. Towards this goal, chromatographic methods have been predominantly used but these require expensive, laboratory-based instrumentation and trained personnel that preclude their implementation in the field for on-site analysis [5]. On the other hand, biosensors offer an alternative and highly attractive approach for antibiotic residue monitoring, due to their portability and low-cost. Amongst the different types of bioreceptors used in various biosensing devices, aptamers (single-stranded oligonucleotides capable of binding to an analyte with high affinity due to the 3D structural arrangement they conform to) present numerous advantages. As a

result, many aptasensors have been already developed for the detection of several antibiotics including OTC [6,7]. Furthermore, the implementation of electrochemical sensing in aptamer-based assay, offers some important advantages such as high sensitivity, low cost and portable equipment, applicability to on-site analysis and scope for miniaturization [8].

Herein, the fabrication and application of electrochemical gold-based aptasensors for the label-free assay of OTC is described. Thin-film gold electrodes were fabricated by sputtering gold on a Kapton film. Subsequently, thiol-modified aptamers were immobilized onto the electrodes, by exploiting the interaction of sulfur with gold. Selective capture of OTC to the aptamer-functionalized electrodes was monitored electrochemically using cyclic voltammetry (CV), differential-pulse voltammetry (DPV) and electrochemical impedance spectroscopy (EIS) and $\text{Fe}(\text{CN})_6^{4-}/\text{Fe}(\text{CN})_6^{3+}$ as a redox probe (Figure 1). The decrease in charge transfer of the redox probe could be related to the OTC concentration.

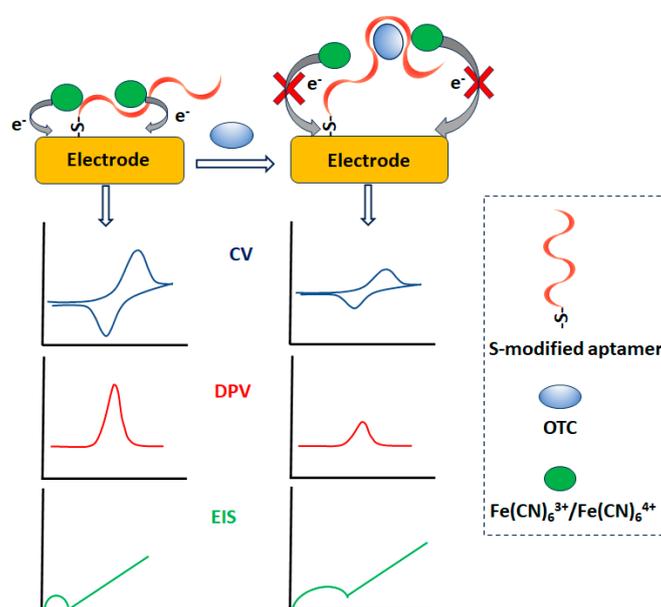


Figure 1. The principle of the aptamer-based assay at the microfabricated gold electrodes.

2. Experimental

2.1. Reagents and Materials

Reagents were of analytical grade and provided from Sigma-Aldrich (Burlington, MA, USA). The aptamer sequence was: 5'-GGA ATT CGC TAG CAC GTT GAC GCT GGT GCC CGG TTG TGG TGC GAG TGT TGT GTG GAT CCG AGC TCC ACG TG/3ThioMC3-D/-3' and was purchased from Integrated DNA Technologies Inc. (IA, USA). The aptamer was diluted in phosphate buffer (PB) (10 mM, pH 7.4), containing 1 mM MgCl_2 . OTC was purchased by Thermo Fisher Scientific (Waltham, MA, USA) and a stock solution of 100 mg/L was prepared in DMSO:PB (50:50 *v/v*).

OTC standard calibration solutions containing 0, 25, 50, 100, 200, 400 and 600 ng/mL of OTC were prepared in PB (pH 7.4). A milk matrix was prepared by dissolving 1.00 g of low-fat dried milk powder in 50 mL of PB (pH 7.4), centrifuging and reconstituting the supernatant solution to a final volume of 10.0 mL with PB. OTC matrix-matched standard calibration solutions containing 0, 25, 50, 100, 200, 400 and 600 ng/mL of OTC were prepared in milk matrix.

A spiked milk sample was prepared as follows: 1.00 g of low-fat dried milk powder was spiked with 10 μg of OTC, dissolved in 50 mL of PB (pH 7.4) and centrifuged; the supernatant solution was reconstituted to a final volume of 10.0 mL with PB.

All electrochemical measurements were performed using a solution containing 5 mM $\text{Fe}(\text{CN})_6^{4-}/\text{Fe}(\text{CN})_6^{3+}$ in 0.1 M KCl.

2.2. Instrumentation

A Metrohm Autolab PGSTAT12 Potentiostat/Galvanostat equipped with the GPES Software (Metrohm, Switzerland) was used for all the electrochemical measurements. Measurements were carried out in a standard electrochemical cell consisting of a Ag/AgCl reference electrode, a Pt counter electrode and the microfabricated thin-film gold electrode as the working electrode. The measurement conditions were: DPV: from -0.1 to $+0.4$ V, scan rate 10 mV/s, step 5 mV, pulse amplitude 25 mV, modulation time 50 ms, interval time 0.5 s; CV: from -0.5 to $+0.5$ V, scan rate 50 mV/s; EIS: DC potential $+0.25$ V, AC potential 10 mV, frequency range $100,000$ Hz to 0.1 Hz.

Circular dichroism (CD) spectra were recorded (200 – 320 nm range, 2 nm bandwidth, 50 nm/min scan rate) using a Jasco J-1500 CD spectrometer (Tokyo, Japan) thermostated at 25 °C.

Sputtering was performed with a CV401 system (Cooke Vacuum Products) and atomic force microscopy (AFM) images were taken with a SPM SMENA instrument.

2.3. Fabrication of the Thin-Film Gold Sensors

The thin-film gold electrodes were fabricated by metal sputtering. A film of flexible Kapton® HN polyimide film (50 μm thicknesses, from RS) was covered with a metal mask with the electrode pattern and Cr and Au were sputtered on the wafer at a nominal thickness of 5 and 100 nm, respectively. Schematic of the fabrication process of the gold sensors and an array of gold electrodes are illustrated in Figure 2a,b, respectively.

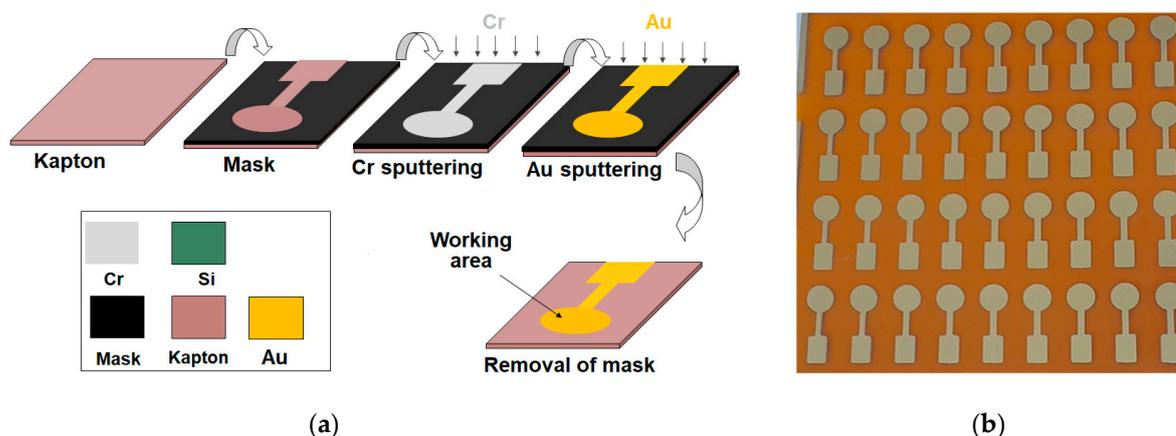


Figure 2. (a) Schematic diagram of the fabrication process of the thin-film gold electrodes, (b) photograph of an array of 36 electrodes.

2.4. Experimental Protocol

The aptamer stock solution was heated for 5 min at 95 °C and allowed to cool down to room temperature. Aptamer solutions of 5 , 10 , 20 and 40 μM were prepared in PB containing 1 mM MgCl₂. 10 μL of the aptamer solution was drop-casted onto the thin-film gold working electrode surface and was left for 12 h at 4 °C in a humidity chamber. The aptamer-modified electrodes were thoroughly-washed with PB to remove unbound aptamers. Subsequently, 5 μL of mercaptoethanol solution (1 mM in $1:2$ (v/v) water/ethanol) was added at the aptamer-modified electrode and was left for 30 min at room temperature.

OTC detection was accomplished by incubating 60 μL of the standard solution or milk sample onto the sensor surface for 30 min at room temperature. Then, the electrode was washed thoroughly with PB to remove unbound OTC and subjected to electrochemical analysis.

3. Results and Discussion

AFM imaging of the thin-film gold electrodes indicates that the gold film is grainy in structure with roughness of ca. 9 nm and grain diameter of c.a. 15 nm (Figure 3a). These data demonstrate an exceptionally smooth surface morphology which is suitable for reproducible and uniform attachment of the aptamer, as opposed to the commonly used thick-film screen-printed gold deposits that exhibit a much rougher surface and, consequently, lower device-to-device uniformity.

The CD spectrum of the aptamer before and after the addition of different concentrations of OTC is illustrated in Figure 3b. The spectrum reveals that the aptamer adopts a parallel G-quadruplex conformation (maximum at 260 nm, minimum at 240 nm), while incubation with increasing OTC concentrations results in a shift of the peak minimum from ca. 240 nm to ca. 250 nm, coupled with a decrease of the peak maximum at ca. 270 nm and the appearance of a peak at ca. 290 nm, indicative of an analyte-induced folding of the aptamer into a hybrid G quadruplex or a mixture of hybrid and antiparallel quadruplexes [9].

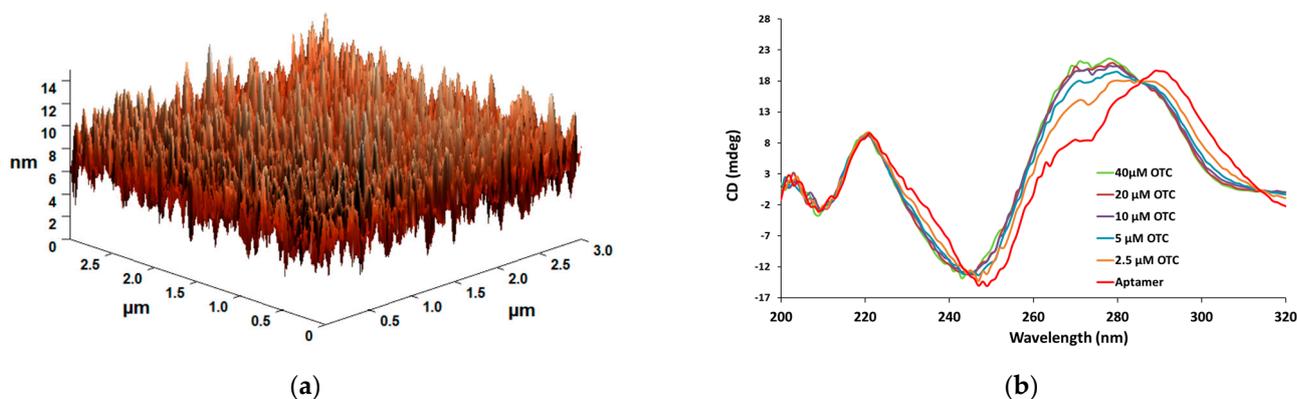


Figure 3. (a) AFM image of the thin-film gold electrode surface, (b) CD spectrum of the aptamer before and after the addition of OTC.

The different steps of the aptasensor preparation and the assay were studied by EIS and CV (Figure 4). EIS demonstrated that the charge transfer resistance of the bare electrode increased upon successive immobilization of the aptamer, mercaptoethanol and OTC (Figure 4a). This was corroborated by the respective CVs which showed that the redox current decreased as the bare electrode was successively treated with aptamer, mercaptoethanol and OTC (Figure 4b). These results suggest that the aptamer is successfully immobilized on the electrode surface and that the OTC is effectively bound to the immobilized aptamer. The concentration of the aptamer was studied and a 20 μM solution was found to produce the highest sensitivity and repeatability.

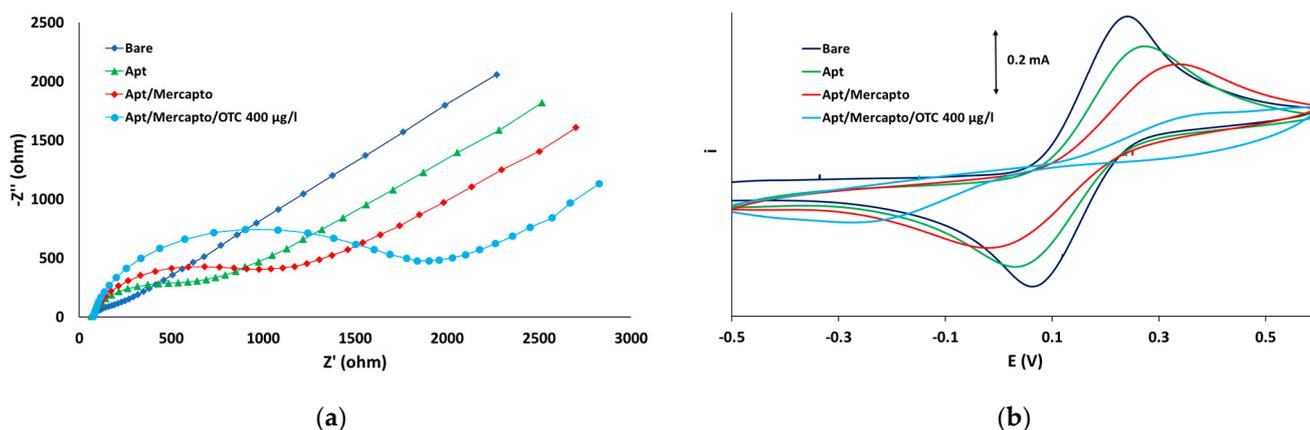


Figure 4. (a) EIS spectra, (b) CVs at a bare gold electrode and gold electrodes after successive immobilization of aptamer, conditioning with mercaptoethanol and incubation with 200 $\mu\text{g/L}$ OTC. Aptamer concentration 20 μM .

Analytical measurements were performed by recording the DPV oxidation current of the $\text{Fe}(\text{CN})_6^{4-}/\text{Fe}(\text{CN})_6^{3-}$ redox probe at different OTC concentrations in the range 0–600 $\mu\text{g/L}$. Increasing concentrations of OTC induced reduction of the DPV current as a result of the aptamer blocking of the electrode surface. The % signal reduction, $I\%$, was calculated as: $I\% = (i_0 - i)/i_0$ (where i_0 is the DPV current at the aptamer-modified electrode in the absence of OTC and i is the DPV current at the aptamer-modified electrode in the presence of OTC).

In order to assess possible milk matrix interference, the matrix effect was calculated as $ME = I\%_{\text{ost}}/I\%_{\text{omm}}$ (where $I\%_{\text{omm}}$ is the signal reduction in a matrix-matched OTC standard and $I\%_{\text{ost}}$ is the signal reduction in the same OTC standard in PB) (Table 1). These data indicate that a more pronounced matrix effect existed at lower OTC concentrations, so that a matrix-matched calibration plot is recommended for quantitative assays.

Table 1. Study of the milk matrix effect.

[OTC] ($\mu\text{g/L}$)	ME
25	1.25
50	1.23
100	1.15
200	1.15
400	1.11
600	1.05

Typical DPV traces are illustrated in Figure 5 and the linear-linear ($I\%_{\text{omm}}$ vs. [OTC]) and linear-log ($I\%_{\text{omm}}$ vs. $\log[\text{OTC}]$) calibration plots are shown as inserts. The limit of detection (LOD) of OTC was ~ 5 $\mu\text{g/L}$ (calculated as the OTC concentration that produced a statistically different signal from the blank). The between-sensors repeatability (calculated as the % relative standard deviation from 5 different aptasensors) was 16% at the 100 $\mu\text{g/L}$ OTC level.

Preliminary experiments were carried out for the determination of OTC in a milk sample spiked with 100 $\mu\text{g/L}$ OTC. The recovery was calculated as $R\% = I\%_{\text{osp}}/I\%_{\text{omm},100}$ (where $I\%_{\text{osp}}$ is the % signal reduction in the spiked milk sample and $I\%_{\text{omm},100}$ is the % signal reduction in a 100 $\mu\text{g/L}$ matrix-matched standard of OTC). The mean recovery ($n = 3$) was calculated as 95%.

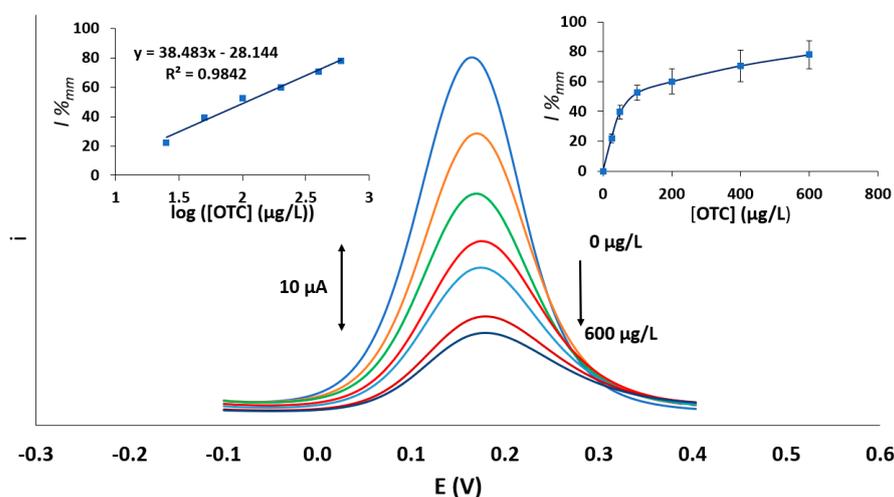


Figure 5. DPV traces obtained with the aptasensor at different matrix-matched OTC standards in the concentration the range 0–600 µg/L. The linear-linear and linear-log calibration plots are shown as inserts.

Author Contributions: Conceptualization, A.E., G.T., J.W., T.S. and Z.K.; methodology, A.E., G.T., J.W., T.S. and Z.K.; validation, V.M., A.A., K.J. and D.S.; investigation, V.M., A.A., K.J. and D.S.; data curation, K.J. and D.S.; writing—original draft preparation, A.E. and D.S.; writing—review and editing, A.E., G.T., J.W. and Z.K.; supervision, A.E., G.T., J.W. and Z.K.; project administration, A.E.; funding acquisition, A.E., G.T., J.W. and Z.K. All authors have read and agreed to the published version of the manuscript.

Funding: This work was supported by the European Union’s Horizon 2020 Research and Innovation Programme under the Marie Skłodowska-Curie Grant Agreement No. 101007299.

Institutional Review Board Statement: Not applicable.

Informed Consent Statement: Not applicable.

Data Availability Statement: Not applicable.

Conflicts of Interest: The authors declare no conflict of interest.

References

1. Landers, T.F.; Cohen, B.; Wittum, T.E.; Larson, E.L. A Review of Antibiotic Use in Food Animals: Perspective, Policy, and Potential. *Public Health Rep.* **2012**, *127*, 4–22. Available online: <http://www.jstor.org/stable/41639470> (accessed on).
2. Virto, M.; Santamarina-García, G.; Amores, G.; Hernández, I. Antibiotics in Dairy Production: Where Is the Problem? *Dairy* **2022**, *3*, 541–564. <https://doi.org/10.3390/dairy3030039>.
3. Commission Regulation (EU) No. 37/2010. Available online: <https://eur-lex.europa.eu/legal-content/EN/TXT/?uri=CELEX%3A32010R0037> (accessed on).
4. Sversut, R.A.; da Silva, A.A.; Mazon Cardoso, T.F.; Kassab, N.M.; do Amaral, M.S.; Nunes Salgado, H.R. A Critical Review of Properties and Analytical Methods for the Determination of Oxytetracycline in Biological and Pharmaceutical Matrices. *Crit. Rev. Anal. Chem.* **2017**, *47*, 154–171. <https://doi.org/10.1080/10408347.2016.12366>.
5. Peris-Vicente, J.; Peris-García, E.; Albiol-Chiva, J.; Durgbanshi, A.; Ochoa-Aranda, E.; Carda-Broch, S.; Bose, D.; Esteve-Romero, J. Liquid chromatography, a valuable tool in the determination of antibiotics in biological, food and environmental samples. *Microchem. J.* **2022**, *177*, 107309. <https://doi.org/10.1016/j.microc.2022.107309>.
6. Mehlhorn, A.; Rahimi, P.; Joseph, Y. Aptamer-Based Biosensors for Antibiotic Detection: A Review. *Biosensors* **2018**, *8*, 54. <https://doi.org/10.3390/bios802005>.
7. Liang, G.; Song, L.; Gao, Y.; Wu, K.; Guo, R.; Chen, R.; Zhen, J.; Pan, L. Aptamer Sensors for the Detection of Antibiotic Residues— A Mini-Review. *Toxics* **2023**, *11*, 513. <https://doi.org/10.3390/toxics11060513>.
8. Evtugyn, G.; Porfireva, A.; Tsekenis, G.; Oravczova, V.; Hianik, T. Electrochemical Aptasensors for Antibiotics Detection: Recent Achievements and Applications for Monitoring Food Safety. *Sensors* **2022**, *22*, 3684. <https://doi.org/10.3390/s22103684>.
9. Kejnovská, I.; Renčíuk, D.; Palacký, J.; Vorlíčková, M. CD Study of the G-Quadruplex Conformation. *Methods Mol. Biol.* **2019**, *2035*, 25–44. https://doi.org/10.1007/978-1-4939-9666-7_2.

Disclaimer/Publisher’s Note: The statements, opinions and data contained in all publications are solely those of the individual author(s) and contributor(s) and not of MDPI and/or the editor(s). MDPI and/or the editor(s) disclaim responsibility for any injury to people or property resulting from any ideas, methods, instructions or products referred to in the content.