



Proceedings

Design of a Fog Computing, Blockchain and IoT-Based Continuous Glucose Monitoring System for Crowdsourcing mHealth [†]

Tiago M. Fernández-Caramés *  and Paula Fraga-Lamas 

Department of Computer Engineering, Faculty of Computer Science, Universidade da Coruña, 15071 A Coruña, Spain; paula.fraga@udc.es

* Correspondence: tiago.fernandez@udc.es; Tel.: +34-981167000 (ext. 6051)

† Presented at the 5th International Electronic Conference on Sensors and Applications, 15–30 November 2018; Available online: <https://ecsa-5.sciforum.net/>.

Received: date; Accepted: date; Published: date



Abstract: Diabetes Mellitus, usually called only Diabetes, is a worldwide chronic metabolic disorder that is characterized by abnormal oscillations in blood sugar levels. Such levels should be monitored by diabetes patients, which traditionally have had to take blood samples by finger-pricking at least between twice and four times a day. Finger-pricking has a number of drawbacks that can be tackled by Continuous Glucose Monitors (CGMs), which are able to determine blood sugar levels throughout the day and not only at specific time instants. In this paper it is proposed the design of an IoT CGM-based system whose collected blood sugar sample values can be accessed remotely, thus being able to monitor patients, specifically dependent ones (e.g., children, elders, pregnant women) and warn them in case a dangerous situation is detected. In order to create such a system, a fog computing system based on distributed mobile smart phones has been devised to collect data from the CGMs. Moreover, it is proposed the use of a blockchain to receive, validate and store the collected data with the objective of avoiding untrusted sources and, thus, provide a transparent and trustworthy data source of a population, which can vary in age, ethnicity, psychology, education, self-care and/or geographic location, in a rapid, flexible, scalable and low-cost way. These crowdsourced data can enable novel mHealth applications for diagnosis, patient monitoring or even public health actions that can help to advance in the control of the disease and raise global awareness on the increasing prevalence of diabetes.

Keywords: diabetes; glucose monitoring; CGM; fog computing; IoT; blockchain; crowdsourcing mHealth; public health; decision support; personalized medicine

1. Introduction

Diabetes Mellitus (DM), usually called only Diabetes, is a worldwide chronic metabolic disorder that is characterized by abnormal oscillations in blood sugar levels. Diabetes is related to diverse illnesses, being involved with certain kinds of blindness and problems in kidneys, blood vessels or heart.

The World Health Organization (WHO) categorizes DM in three different types [1]: Type-1 DM, Type-2 DM and gestational diabetes. Type-1 DM patients need insulin on a daily basis, since their body is not able to produce it properly. Type-2 DM is the most common and occurs when the body makes an ineffective use of insulin. Until recently, Type-2 DM was mostly observed in adults, but currently, largely due to overweight and the lack of physical activity, it is increasingly occurring in children. Regarding gestational diabetes, it is characterized by above normal blood sugar levels in women during pregnancy.

Due to the characteristics of DM, it is important to monitor vulnerable groups, especially children, the elderly and pregnant women. Such a monitoring has been traditionally performed by taking blood samples through finger-pricking, which has a number of drawbacks (e.g., active involvement of the patient/care taker, infections) that can be tackled by Continuous Glucose Monitors (CGMs), which are based on a small device with a sensor that takes blood sugar readings 24 h a day. Such measurements make it easier for diabetics to have more precise control over blood sugar and allow for making informed decisions regarding a potential treatment on a patient. Thus, CGMs may warn patients about glucose highs and lows in order to take the appropriate preventive measures.

The concept of CGM opens the possibility of creating Internet of Things (IoT) devices that provide rapid warnings and take autonomous decisions that need to be performed as fast as possible. Thus, an IoT CGM can make use of a remote cloud system where information is stored and where decisions can be taken according to rules (e.g., to warn a doctor when the patient's blood sugar level is above a specific threshold). However, a cloud computing based architecture have certain limitations: all the information and decisions are centralized are managed, in general, by a third party; the cloud availability may be compromised by its massive use or by cyber-attacks; and, due to the physical distance between patient and cloud, decisions require some time to be taken and communicated, which may be too high in some scenarios. Fortunately, for such scenarios where a fast response and low communications overhead are required, other paradigms have proved to be successful by moving computing capabilities from the cloud towards the edge of the network [2]. One of such paradigms is fog computing, which transfers the cloud's computational and communication capabilities close to the sensor nodes in order to minimize latency, to distribute computational and storage resources, to enhance mobility and location awareness, and to ease network scalability while providing connectivity among devices in different physical environments [3,4].

Another problem found when collecting and processing the sensed data from IoT devices is their security and trustworthiness. Regarding security, diverse authors have proposed energy-efficient mechanisms to make use of high-security cipher suites in IoT devices [5], since they are usually constrained in terms of computational resources, especially when they rely on batteries. With respect to trustworthiness, it is essential when data are shared with third parties. Therefore, the data collected for doctors or for an autonomous system that acts upon the received blood sugar values should be valid.

Crowdsourcing is a distributed problem-solving, knowledge management and production model that takes advantage of the collective intelligence of an online community to research and develop innovative approaches and novel products and services. Its use within public health is starting to being explored [6], specially with the upraise of mobile health (mHealth) which enables healthcare through applications delivered using mobile phones and wireless technologies.

Traditionally, human intelligence-based crowdsourcing mHealth systems have managed the demands of patients and public health stakeholders in a centralized way, hence they are prone to attacks and have an inherent single point of failure. Moreover, user's sensitive information is saved in a database that is exposed to data breaches and data loss.

In contrast, this paper proposes the use of a blockchain-based decentralized framework that does not rely on any central third party and guarantees the users' privacy. In addition, it is described the design of an IoT CGM-based system whose collected blood sugar sample values can be accessed remotely, thus being able to monitor patients, specifically dependent ones (e.g., children, elders, pregnant women) and warn them in case a dangerous situation is detected. In order to create such a system, a fog computing system based on distributed mobile smart phones has been devised to collect data from the CGMs.

2. Related Work

During the last decade different authors studied the use of CGMs in order to apply them to different scenarios. For instance, in [7] it is analyzed the possibility of adding intelligence to CGM sensors in order to issue alerts when glucose levels are not within the appropriate range. The authors

emphasize the fact that sensors have to be calibrated and that their data needs to be filtered to improve their signal-to-noise ratio. The same authors focused later on the same concepts in another paper that reviews the state of the art on contributions to the development of hardware and smart algorithms for CGMs [8]. Similar reviews on the evolution of CGM technology can be found in [9,10].

Other researchers analyzed specific aspects of the CGMs. For example, in [11] the authors studied the problem of calibration algorithms in commercial CGMs and the process of estimating the amount of glucose in blood plasma. Another study [12] highlighted the ability of CGMs to detect losses in the performance on insulin infusion set actuation, which can lead to dangerous complications in Type-1 DM diabetics due to prolonged hyperglycemia.

CGMs have also allowed for studying how daily habits affect diabetics. For instance, in [13] it is reviewed the impact of physical exercise on blood sugar levels on Type-1 DM patients, concluding that even certain daily activities alter the dynamics of glucose and can cause problems with blood glucose regulation during and after exercise.

Finally, it is worth pointing out that, very recently, the IEEE introduced a draft on the part 10425 of its standard IEEE 11073 [14], which is aimed at standardizing the communication between CGMs and between a CGM and other devices (e.g., cell phones, computers, health appliances) in a manner that enables plug-and-play interoperability.

3. Design and Implementation of the System

3.1. Communications Architecture

Figure 1 shows the proposed communications architecture. In such a figure, CGM sensors collect blood sugar levels from multiple patients and send them to smartphones that run a mHealth fog service. The fog service collects and processes the data (depending on the sensed values, the service decides the measures to be taken). Moreover, the fog service is able to send the processed values and additional information on the patients to both a remote server and to the blockchain, where they are stored.

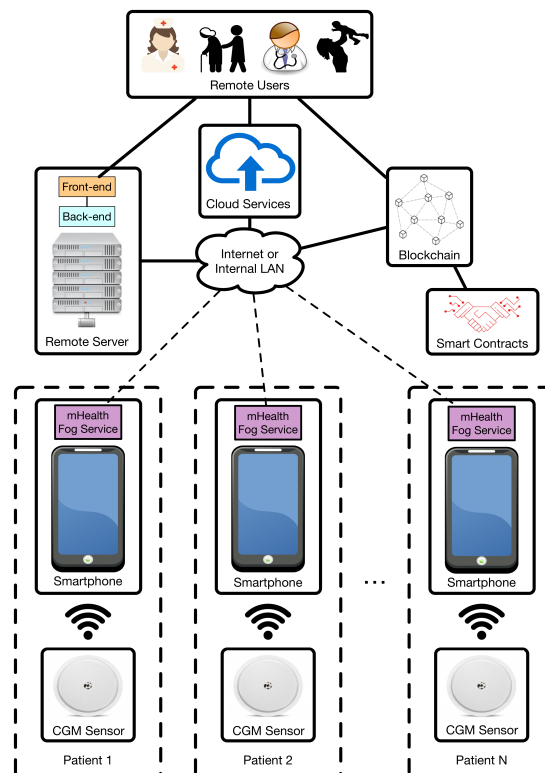


Figure 1. Communications architecture.

In the case of the remote server, it basically makes use of a back-end that collects the sensed values and a front-end that displays them in a user-friendly way through a web interface to remote users like doctors, nurses or children/elderly care takers.

Regarding the type of blockchain, a federated blockchain was selected to increase the transaction privacy and accelerate the transaction validation. Only registered and authorized users can access to the network and the consensus algorithm is run by a pre-selected group of nodes. The federated blockchain stores the received data or their unique hashes, enabling public access to them in a secure way. Data anonymization of the patients can also be included to protect their privacy (i.e., to guarantee that there is not a link with the real identity of a patient). In addition, the blockchain can run smart contracts, so, for instance, when it is detected that a user is going to run out of sensors, an automated purchase can be performed.

3.2. Implementation

In order to implement a first proof-of-concept version of the proposed system, the following components, which are shown in Figure 2, were selected:

- CGM Sensor: Abbott's Freestyle Libre. Although its reading range is limited (up to 20 cm) due to the use of NFC, its sensors last longer than others provided by Dexcom or Medtronic (14 days versus roughly a week), it is a cost-effective solution (e.g., a kit with one reader and sensors currently costs € 169.69), finger-pricking is not necessary on a daily basis to calibrate the sensor and it is more accurate than other systems (i.e., it has lower Mean Absolute Relative Difference (MARD)).
- Cloud service: Nightscout. It is an open-source system aimed at collecting CGM data through a cloud service that is also able to display them through a web interface.
- Smartphone apps. Glimp is used to read Abbott's Freestyle Libre CGM sensor through NFC. A lightweight Ethereum client can also run on the smartphone and a monitoring fog app may read the blood sugar values and decide whether it is necessary to take certain actions (e.g., warn the patient or his/her care takers) without relying on cloud services.
- Back-end and front-end: Django. It is a framework based on Python that allows for developing web applications fast. In addition, the proposed system makes use of SQLite3 as database and a HTML/Javascript for the web page displayed by the front-end.
- Blockchain and smart contracts [15]: Ethereum. It is an open-source platform based on blockchain technology that is able to run smart contracts.
- Warning system: Twilio and Telegram. Although, for clarity purposes, this system is actually not depicted in Figure 2, it is essential when sending warnings to remote users to their smartphone. Thus, Twilio allows the system to send custom SMS, while it was programmed a Telegram bot to send instant messages.

The regular functioning of the system is quite straightforward. After the sensor has been placed on the patient arm, it has to be read periodically by approaching the smartphone. The read values can be uploaded both to Nightscout or Ethereum, where they may be accessed by remote users. When the read values exceed a prefixed threshold (specified through the managing web application that runs on the front-end), the system sends warnings fast to the patient or to his/her caretakers. Regarding the information stored in Ethereum, depending on the scenario, it can be accessed by remote users of the public Ethereum blockchain or by a selected group of users that run an internal blockchain. In both cases, besides storing the relevant data, smart contracts coded in Solidity can be run on the blockchain.

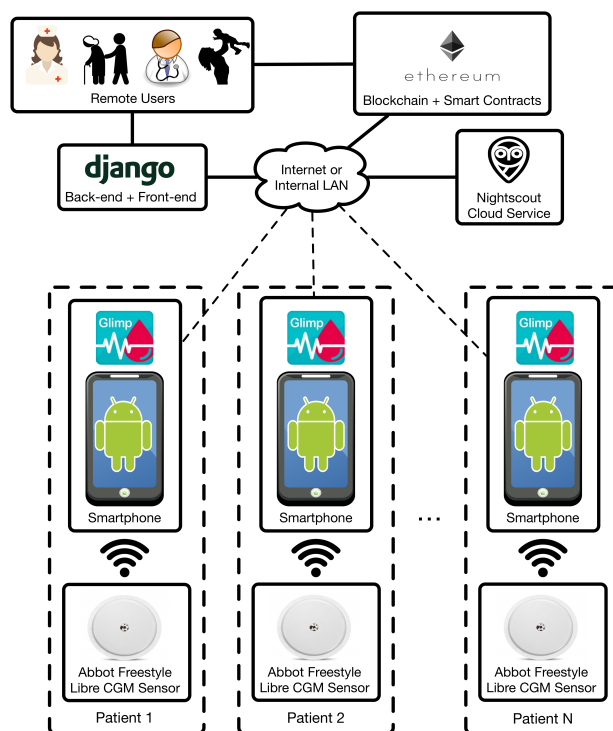


Figure 2. Implemented system.

3.3. Preliminary Results

Although the presented system still needs to be enhanced (for instance, in this first implemented version, smart contracts were not deployed on the blockchain), the basic functionality of the system was tested on a patient for 14 days. As an example, Figure 3 shows a snapshot of one of the menus of the web front-end that depicts the collected blood sugar level values. The system has been already proved to be useful since, as it is pointed out by the orange circle in Figure 3, it has been able to detect and warn the patient in advance regarding a sudden descent in blood sugar level that anticipated a hypoglycemia.




Figure 3. Blood sugar levels measured on a patient during the first week.

4. Conclusions

In this paper it was presented the design and a preliminary version of an IoT CGM-based system for crowdsourcing mHealth. Such a system is able to collect blood sugar levels from remote CGMs that can be accessed remotely. Therefore, the system allows for monitoring patients and warn them in case a dangerous situation is detected. In order to create such a system, a fog computing system based on distributed mobile smart phones was devised to collect data from the CGMs and send them to a remote cloud and/or to a blockchain. Thanks to the blockchain and the proposed CGM-based system it is possible to provide a transparent and trustworthy blood sugar data source from a population in a rapid, flexible, scalable and low-cost way. Such crowdsourced data can enable novel mHealth

applications for diagnosis, patient monitoring or even public health actions that may help to advance in the control of the disease and raise global awareness on the increasing prevalence of diabetes.

Acknowledgments: This work has been funded by the Xunta de Galicia (ED431C 2016-045, ED341D R2016/012, ED431G/01), the Agencia Estatal de Investigación of Spain (TEC2013-47141-C4-1-R, TEC2015-69648-REDC, TEC2016-75067-C4-1-R) and ERDF funds of the EU (AEI/FEDER, UE). The work of P. Fraga-Lamas was supported in part by BBVA and the BritishSpanish Society Grant. The authors would like to acknowledge the collaboration of Manuel Pérez Parada testing the Abbott FreeStyle Libre CGM system during his bachelor's thesis.

References

1. World Health Organization. Diabetes: Key Facts. Available online: <http://www.who.int/news-room/fact-sheets/detail/diabetes> (accessed on October 2018)
2. Markakis, E.K.; Karras, K.; Zotos, N.; Sideris, A.; Moysiadis, T.; Corsaro, A.; Alexiou, G.; Skianis, C.; Mastorakis, G.; Mavromoustakis, C.X.; et al. EXEGESIS: Extreme Edge Resource Harvesting for a Virtualized Fog Environment. *IEEE Commun. Mag.* **2017**, *55*, 173–179.
3. Bonomi, F.; Milito, R.; Zhu, J.; Addepalli, S. Fog Computing and its Role in the Internet of Things. In Proceedings of the First Edition of the MCC Workshop on Mobile Cloud Computing, Helsinki, Finland, 13–17 August 2012; pp. 13–16.
4. Fernández-Caramés, T.M.; Fraga-Lamas, P.; Suárez-Albela, M.; Díaz-Bouza, M.A. A Fog Computing Based Cyber-Physical System for the Automation of Pipe-Related Tasks in the Industry 4.0 Shipyard. *Sensors* **2018**, *18*, 1961.
5. Suárez-Albela, M.; Fernández-Caramés, T.M.; Fraga-Lamas, P.; Castedo, L. A Practical Evaluation of a High-Security Energy-Efficient Gateway for IoT Fog Computing Applications. *Sensors* **2017**, *9*, 1978.
6. Brabham, D.C.; Ribisl, K.M.; Kirchner, T.R.; Bernhardt, J.M. Crowdsourcing Applications for Public Health. *Am. J. Prev. Med.* **2014**, *46*, 179–187.
7. Sparacino, G.; Facchinetti, A.; Cobelli, C. 'Smart' Continuous Glucose Monitoring Sensors: On-Line Signal Processing Issues. *Sensors* **2010**, *10*, 6751–6772.
8. Facchinetti, A. Continuous Glucose Monitoring Sensors: Past, Present and Future Algorithmic Challenges. *Sensors* **2016**, *16*, 2093.
9. Cappon, G.; Acciaroli, G.; Vettoretti, M.; Facchinetti, A.; Sparacino, G. Wearable Continuous Glucose Monitoring Sensors: A Revolution in Diabetes Treatment. *Electronics* **2017**, *6*, 65.
10. Chen, C.; Zhao, X.-L.; Li, Z.-H.; Zhu, Z.-G.; Qian, S.-H.; Flewitt, A.J. Current and Emerging Technology for Continuous Glucose Monitoring. *Sensors* **2017**, *17*, 182.
11. Rosetti, P.; Bondia, J.; Vehí, J.; Fanelli, C.G. Estimating Plasma Glucose from Interstitial Glucose: The Issue of Calibration Algorithms in Commercial Continuous Glucose Monitoring Devices. *Sensors* **2010**, *10*, 10936–10952.
12. Howsmon, D.P.; Cameron, F.; Baysal, N.; Ly, T.T.; Forlenza, G.P.; Maahs, D.M.; Buckingham, B.A.; Hahn, J.; Bequette, B.W. Continuous Glucose Monitoring Enables the Detection of Losses in Infusion Set Actuation (LISAs). *Sensors* **2017**, *17*, 161.
13. Ding, S.; Schumacher, M. Sensor Monitoring of Physical Activity to Improve Glucose Management in Diabetic Patients: A Review. *Sensors* **2016**, *16*, 589.
14. IEEE. *IEEE Approved Draft—Health Informatics—Personal Health Device Communication—Part 10425: Device Specialization—Continuous Glucose Monitor (CGM)*; IEEE: Piscataway, NJ, USA, 2017.
15. Fernández-Caramés, T.M.; Fraga-Lamas, P. A Review on the Use of Blockchain for the Internet of Things. *IEEE Access* **2018**, *6*, 32979–33001.



© 2018 by the authors. Licensee MDPI, Basel, Switzerland. This article is an open access article distributed under the terms and conditions of the Creative Commons Attribution (CC BY) license (<http://creativecommons.org/licenses/by/4.0/>).