

Proceedings

Human Periodontal Ligament Characterization by Means of Vibrational Spectroscopy and Electron Microscopy

Carlo Camerlingo ¹, Fabrizia d'Apuzzo ², Marcella Cammarota ³, Sonia Errico ³, Marianna Portaccio ³, Letizia Perillo ² and Maria Lepore ^{3,*}

¹ CNR-SPIN, Istituto Superconduttori, Materiali Innovativi e Dispositivi, via Campi Flegrei 34, Pozzuoli 80078, Italy

² Dip. Multidisciplinare di Specialità Medico-Chirurgiche e Odontoiatriche, Università degli Studi della Campania *Luigi Vanvitelli*, via L. De Crecchio 6, Napoli 80138, Italy

³ Dip. di Medicina Sperimentale, Università degli Studi della Campania *Luigi Vanvitelli*, via S. Maria di Costantinopoli 16, Napoli 80138, Italy

* Correspondence: maria.lepore@unicampania.it

† Presented at the 7th Electronic Conference on Sensors and Applications, 15–30 November 2020; Available online: <https://ecsa-7.sciforum.net/>.

Published: 15 November 2020

Abstract: Human periodontal ligament (PDL) is a membrane-like connective tissue interposed between the tooth root and the alveolar bone of which the main component is represented by collagen fibers. During the early stage of application of orthodontic forces different changes occur in PDL. For this reason, its characterization with conventional and non-conventional techniques can be extremely interesting. We investigated samples of PDL of orthodontic patients, aged between 13 and 21 years, using different experimental techniques. Morphological characterization of PDL samples was carried out by using a scanning electron microscope. Fourier Transform Infrared (μ -FT-IR) and Raman (μ -RS) microspectroscopies were used for biochemical characterization of PDL samples. A biochemical characterization of PDL tissues with clear evidence of contributions from collagen, lipid and other protein was obtained. The analysis of Amide I and Amide III components was also performed giving indication on the protein secondary structure.

Keywords: Periodontal ligament; gingival crevicular fluid; Raman microspectroscopy; Fourier-Transform infrared microspectroscopy

1. Introduction

The periodontal ligament (PDL) is the structure interposed between the tooth root and the alveolar bone, occupying an area of 0.25 to 0.5 mm². It is a connective tissue whose main component is represented by a set of collagen elastic fibers, parallel to each other, which are inserted on one side in the cementum and on the other in the lamina dura of the alveolar bone (Sharpey's fibers). The oblique direction of these support fibers in their attack on the tooth surface allows the tooth to possess an elasticity enough to distribute the masticatory forces over a large surface of the alveolar process, allowing the tooth to oppose a greater resistance to forces exerted during normal chewing. Two other important components of the periodontal ligament are: cellular elements, consisting of undifferentiated mesenchymal cells and their lines of differentiation in fibroblasts and osteoblasts, together with the neural elements, and vascular tissue fluid from the circulatory system. The periodontal ligament has vessels and cells of the blood system, despite the poor vascularization and innervation characterized by amyelinic nerves appointed to nociceptive perception, and receptors

associated with proprioception, responsible of the perception of the position of the tooth into alveolus and the spatial relationship between the jaws during mastication [1,2]. PDL plays a relevant role during orthodontic treatment and for this reason it is interesting to characterize its structure and components. In the present manuscript, samples of PDL obtained before any orthodontic treatment have been examined by using different experimental techniques that can offer complementary information on PDL properties. Scanning electron microscopy has been used for investigating PDL structures, while Fourier transform Infrared microspectroscopy (μ -FT-IR) and Raman microspectroscopy (μ -RS) allowed us to characterize PDL from a biochemical point of view.

2. Materials and Methods

2.1. Sample Preparation

Samples of periodontal ligaments (PDL) of orthodontic patients; aged between 13 and 21 years, and treated with extraction of upper and/or lower premolars, have been selected. Informed consent was obtained from each minor patient's parents or adult patients after providing them detailed information about the clinical trial. The PDL was scarified from radicular surface of the extracted premolars using a one-way lancet. Each sample has dimensions of the order of few mm³. The PDL samples were fixed in 4% paraformaldehyde (PFH) at least in 3 h. PFH was removed by centrifugation (2000 rpm for 2 min). To fix samples graded series of ethanol solutions (50%–70%–80%–95%) were used. Samples were leaved in each ethanol's solution for 1 h at room temperature starting from 50% solution to 95% and then they were stored in ethanol 100% until analysis.

2.2. Experimental Techniques

2.2.1. Scanning Electron Microscopy (SEM)

Collected PDL samples were washed in PBS, fixed in 4% paraformaldehyde in PBS and then dehydrated with increasing ethanol percentage (30–90% in water for 5 min, twice 100% for 15 min). After drying in Critical Point Dryer (EMITECH K850), samples were sputter coated with platinum-palladium (Denton Vacuum DESKV, 77 mAmps e 120 sec.) and observed with Supra 40 Zeiss Field-emission scanning electron microscope (EHT = 5.00 kV, WD = 22 mm, detector in lens).

2.2.2. FT-IR Microspectroscopy

FT-IR spectra were obtained using a Perkin Elmer Spectrum One spectrometer in a transmission geometry using KBr pellets. Initially, 0.1 g of a PDL sample was mixed with 5 mL water and sonicated on ice for 5 min by using a Soniprep 150 Plus Ultrasonic Disregator. The homogenate was stored at -20 °C for 24 h. After this, the sample was lyophilized (24 h), using a Lio-5P Freeze Dryer. KBr pellets were prepared by mixing a small quantity of PDL sample with KBr (at the ratio of 1/100). For every sample two KBr pellets were prepared. All spectra were obtained using 64 scans in the range from 4000 to 450 cm⁻¹ with a 4 cm⁻¹ spectral resolution. The spectra were preliminarily analyzed using the application routines provided by the software package ("Spectrum" Perkin Elmer Inc., Hopkinton, MA, USA) controlling the whole data acquisition system. The spectra were further analyzed in terms of convoluted peak functions to determine the basic vibrational modes that contribute to the FT-IR signal by using a best-fit peak fitting routine of GRAMS software based on the Levenberg-Marquardt nonlinear least square method. Lorentzian-Gaussian curves were used. Peaks constituting the spectrum were manually selected to define the starting conditions for the best-fit procedure. The bestfit was then performed to determine the optimized intensity, position, and width of the peaks. The performance of the procedure was evaluated by means of the χ^2 parameter [3].

2.2.3. Raman Microspectroscopy

Samples were excited by the light of a He-Ne laser operating at a wavelength $\lambda = 633$ nm, with a maximum nominal power of 17 mW. The signal was collected by a *Jobin-Yvon TriAx 180* monochromator, equipped with a liquid N₂ cooled CCD and a grating of 1800 grooves/mm, allowing a spectral resolution of 4 cm⁻¹. The laser light was focused on the sample surface by means of a 100 × (n.a. = 0.90) optical objective on an excitation area of about 10 μm of size. The spectra were obtained using accumulation times ranging in 60–300 s. The spectra were analyzed using the same approach previously described for FT-IR spectra [see also Ref. 4]. For Raman spectra Lorentzian peak shape was used. The band of amide I (located in the 1550- to 1750-cm⁻¹ wave number region) was detailly analyzed for obtaining significant information about protein configuration.

3. Results and Discussion

3.1. SEM Observations

Numerous collagen fibres thickened in bundles are clearly visible at scanning electron microscopy observation as shown in Figure 1A. Figure 2B,C shows in two different area and at different magnification the connection between collagen fibers of periodontal ligament and bone matrix fibres (white asterisk).




Figure 1. SEM micrographs of periodontal ligaments. Collagen fibers and bone matrix. Scale Bar = 1 μm in (A), 2 μm in (B) and (C).

3.2. FT-IR Results

In Figure 2 a representative infrared spectrum of PDL is reported together with the results of the deconvolution procedure performed by using Lorentzian-Gaussian curves. The main contribution to the spectrum and the related assignments are reported in Table 1a. The region related to C-H bonds in the region 3100–2800 cm⁻¹ can be related to collagen contribution evidenced by SEM micrographs and to a lesser extent to lipid content. In the 1750–1000 cm⁻¹ region, the band at 1656 cm⁻¹ is due to the C=O stretching of Amide I. For other peaks see Table 1a. Interesting information about the secondary structure of protein content could be obtained by considering the subcomponents of Amide I and Amide III regions. The deconvolution of Amide I region (1750–1580 cm⁻¹) indicates the presence of different subcomponents that are related to the protein secondary structure. The contributions at 1673 cm⁻¹ is ascribed to β-turn subcomponent, the ones at 1661 and 1650 cm⁻¹ are related to α-helix subcomponent, and the features at 1639 and 1631 cm⁻¹ are due β-sheets subcomponent.




Figure 2. Representative FT-IR spectrum of PDL in the 3100–1000 cm^{-1} with the deconvolution analysis of peaks with Gaussian- Lorentzian curves (blue line: experimental curve).

3.3. Raman Microspectroscopy Results

In Figure 3 a representative Raman spectrum of PDL is reported. As is evident the main contribution due to Amide I and Amide III are evident together with the contributions due to the C-H bonds. These features are related to collagen structure and the bands in the CH_3/CH_2 region could be also associated with tissue lipid components. See Ref. [5] and Table 1b for other assignments and details.

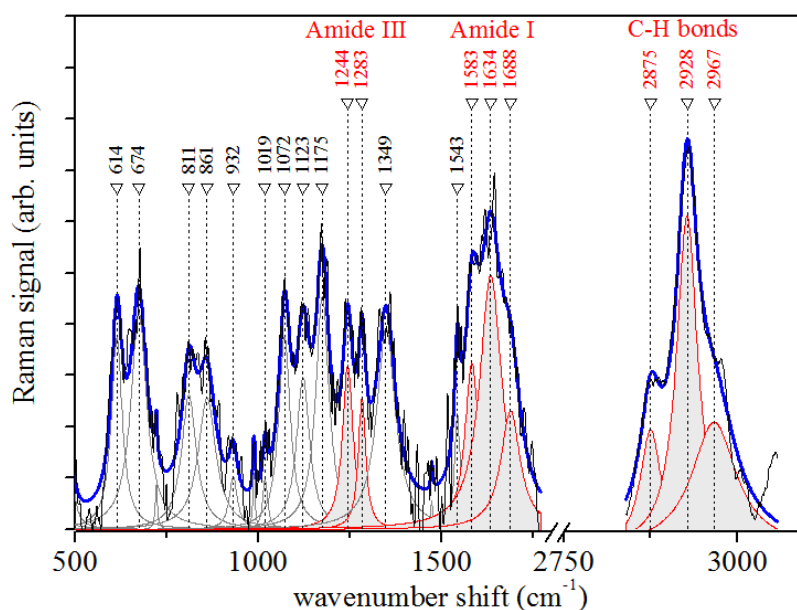


Figure 3. Representative Raman spectrum of PDL. The blue curve is the convolution of the Lorentzian components estimated by fitting the experimental data.

Also in the case of Raman microspectroscopy, the analysis of subcomponents of Amide I and Amide III has allowed us information about the secondary structures of PDL protein content [5,6].

Table 1. Assignments of the main modes of FT-IR (a) and Raman (b) spectra of PDL according to References reported in [3,4].

(a)		(b)	
FT-IR Mode		Raman Mode	
ν (cm ⁻¹)	Assignments	ν (cm ⁻¹)	Assignments
3279	Amide A (-N-H ν)	614	phosphate δ
2960	CH ₃ as. ν	811	CC skeleton
2926	CH ₂ as. ν	861	proline
2873	CH ₃ s. ν	932	phosphate
2850	CH ₂ s. ν	1019	C-N proline
1652	Amide I (C=O ν , C-N ν)	1072	C-N proline
1544	Amide II (C-N ν , C-NH δ , α -helix)	1123	C-N
1455	CH ₃ as. δ , CH ₂ s.	1175	C-O ν
1408	COO ⁻ s. ν	1244	random coil – Amide III
1239	PO ₂ ⁻ as. ν C-O-P ν	1283	α -helix – Amide III
1079	PO ₂ ⁻ s. ν C-O-P ν	1349	CH ₂ Glycine – Amide III
1035	C-O ν	1543	N-H δ – Amide II
		1583	β -sheet – Amide I
		1634	α -helix – Amide I
		1688	β -turn – Amide I
		2875	CH ₂ as. ν
		2928	CH ₃ s. ν
		2967	CH ₃ as. ν

As said before, the Amide I band consisted of major components that are related to the secondary structure of the protein. This band allowed us to obtain information on collagen which is the main PDL component. In particular, the contributions of α helix, β -sheet, collagen 3_{10} -helix and β -turn subcomponent were centered at about 1642, 1647, 1617 and 1668 cm⁻¹, respectively.

4. Conclusions

The reported results highlight the great potential of the techniques used for characterizing human PDL samples from different points of view. In particular, SEM investigation evidences the PDL structure, while μ -FT-IR and μ -RS offer complementary information about biochemical composition of this kind of tissue that plays a very peculiar role during orthodontic treatments when the application of forces can cause structural and biochemical changes.

Author Contributions: Conceptualization, M.L. and L.P.; methodology, C.C., M.P. and M.C.; software, C.C., M.P. and M.C.; investigation, C.C., M.P., M.C. and S.E.; writing—original draft preparation, M.L., C.C. and M.P.; writing—review and editing, M.L., C.C., and M.P. All authors have read and agreed to the published version of the manuscript.

Funding: This research received no external funding

Conflicts of Interest: The authors declare no conflict of interest.

References

1. Anastasi, G.; Cordasco, G.; Matarese, G.; Rizzo, G.; Nucera, R.; Mazza, M.; Militi, A.; Portelli, M.; Cutroneo, G.; Favalaro, A. An immunohistochemical, histological, and electron-microscopic study of the human periodontal ligament during orthodontic treatment. *J. Mol. Med.* **2008**, *21*, 545–554.
2. d'Apuzzo, F.; Cappabianca, S.; Ciavarella, D.; Monsurrò, A.; Silvestrini-Biavati, A.; Perillo, L. Biomarkers of Periodontal tissue remodeling during orthodontic tooth movement in mice and men: Overview and clinical relevance. *Sci. World J.* **2013**, *2013*, 105873.
3. Portaccio, M.; d'Apuzzo, F.; Perillo, L.; Grassia, V.; Errico, S.; Lepore, M. Infrared microspectroscopy characterization of gingival crevicular fluid during orthodontic treatment. *J. Mol. Struct.* **2019**, *1176*, 847–854.
4. Delfino, I.; Perna, G.; Lasalvia, M.; Capozzi, V.; Manti, L.; Camerlingo, C.; Lepore, M. Visible micro-Raman spectroscopy of single human mammary epithelial cells exposed to X-ray radiation. *J. Biomed. Optic.* **2015**, *20*, 035003.
5. Perillo, L.; D'Apuzzo, F.; Illario, M.; Laino, L.; Di Spigna, G.; Lepore, M.; Camerlingo, C. Monitoring Biochemical and structural changes in human periodontal ligaments during orthodontic treatment by means of micro-Raman spectroscopy. *Sensors* **2020**, *20*, 497, doi:10.3390/s20020497.
6. Camerlingo, C.; d'Apuzzo, F.; Grassia, V.; Perillo, L.; Lepore, M. Micro-Raman spectroscopy for monitoring changes in periodontal ligaments and gingival crevicular fluid. *Sensor* **2008**, *14*, 22552–22563.



© 2020 by the authors. Submitted for possible open access publication under the terms and conditions of the Creative Commons Attribution (CC BY) license (<http://creativecommons.org/licenses/by/4.0/>).